
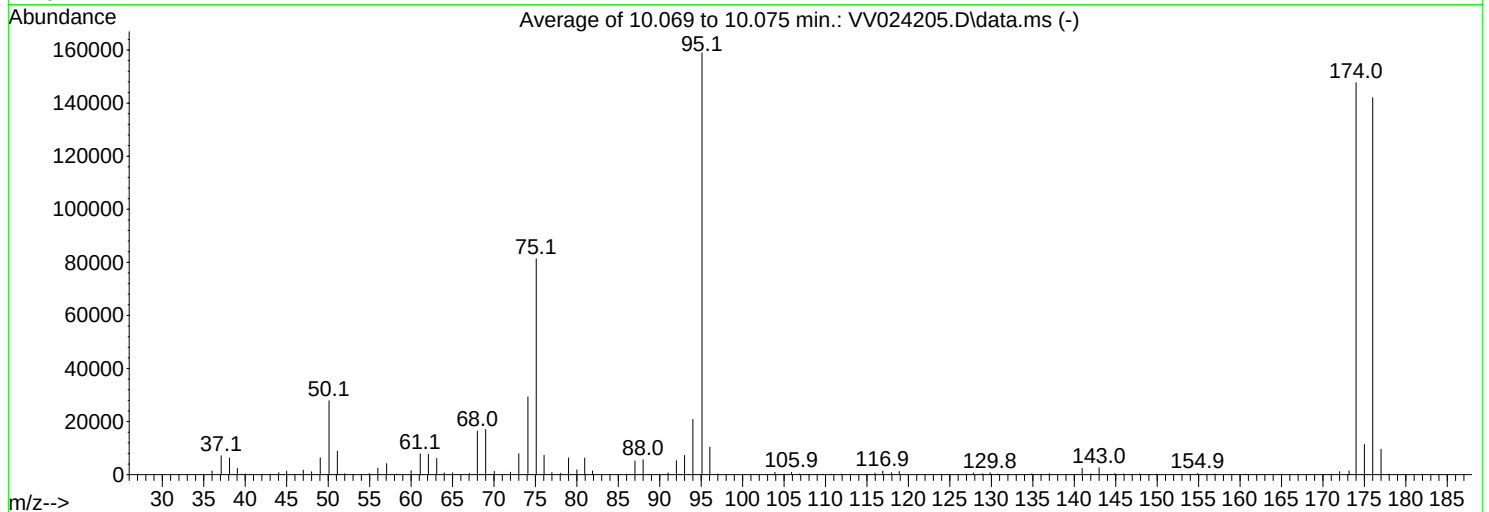


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024205.D
Acq On : 28 Dec 2021 09:06
Operator : SY/MD
Sample : BFB257
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB257

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 31 03:39:03 2021

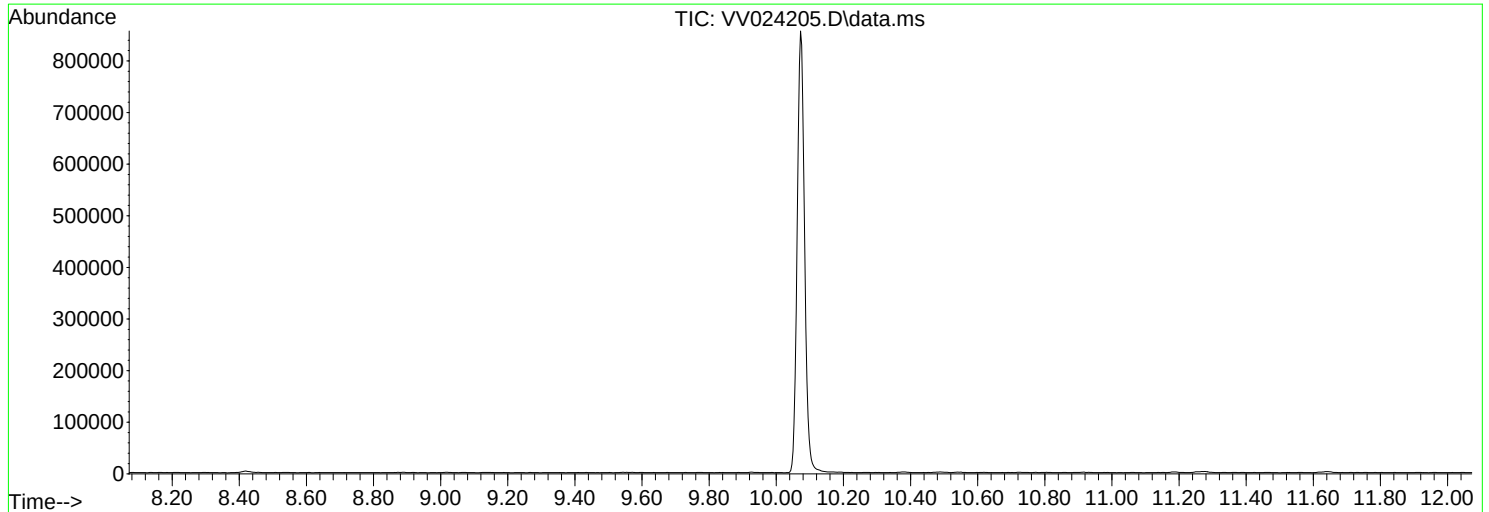

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	27872	PASS
75	95	30	80	51.2	81352	PASS
95	95	100	100	100.0	158933	PASS
96	95	5	9	6.5	10373	PASS
173	174	0.00	2	1.0	1422	PASS
174	95	50	120	92.9	147712	PASS
175	174	5	9	7.7	11362	PASS
176	174	95	105	96.1	142016	PASS
177	176	5	10	6.8	9590	PASS

m/z	Abundance
40.00	2371.0
44.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
36.00	1258.0
37.10	6930.0
38.10	6254.0
39.00	2320.0
40.00	2714.0
43.10	177.0
44.10	930.0
45.00	1216.0
45.90	168.0
47.00	1481.0
48.00	1055.0
49.10	6139.0
50.10	26976.0
51.10	8592.0
52.00	366.0
53.00	101.0
54.90	443.0
56.00	2539.0
57.00	4061.0
58.20	203.0
60.00	1528.0
61.10	7556.0
62.10	7560.0
63.10	6129.0
64.00	672.0
65.00	728.0
66.00	135.0
67.00	402.0
68.00	16183.0
69.00	16720.0
70.10	1331.0
72.00	865.0
73.00	7451.0
74.10	28568.0
75.10	78640.0
76.10	7034.0
77.00	776.0
78.10	615.0
79.00	6119.0
80.00	1789.0
80.90	6153.0
81.90	1274.0
83.10	125.0
86.00	192.0
87.00	4903.0
88.00	5375.0
91.00	636.0
92.00	5025.0
93.00	7065.0
94.00	19792.0
95.10	152448.0
96.00	10279.0
97.00	332.0
103.90	772.0
105.00	238.0
105.90	890.0
106.80	269.0
109.70	152.0
110.70	163.0
111.90	182.0
112.90	154.0
114.90	186.0
115.90	578.0
116.90	1364.0
117.90	796.0
118.90	1092.0
123.80	110.0
127.80	598.0
128.90	308.0
129.90	670.0
130.80	259.0
134.90	369.0
137.00	351.0
140.10	198.0
140.90	2194.0
141.90	244.0
143.00	2357.0
144.00	170.0
144.90	457.0
146.00	273.0
146.90	110.0
147.90	378.0
148.70	150.0
149.90	226.0
151.80	149.0
152.90	131.0
154.90	500.0
157.00	290.0
158.80	172.0
160.70	144.0
170.70	212.0
171.20	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

172.00	1317.0
173.10	1998.0
174.00	139136.0
175.00	11059.0
176.00	133248.0
177.00	9211.0
178.00	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
36.00	1401.0
37.10	7364.0
38.10	6479.0
39.10	2465.0
40.00	2778.0
43.10	165.0
44.10	932.0
45.00	1401.0
46.00	145.0
47.00	1805.0
48.00	1182.0
49.00	6494.0
50.10	28864.0
51.10	9168.0
52.00	336.0
54.90	444.0
56.00	2547.0
57.10	4321.0
58.30	231.0
60.00	1507.0
61.10	8107.0
62.10	8000.0
63.10	6354.0
64.00	679.0
65.00	766.0
65.90	143.0
67.10	464.0
68.00	17024.0
69.00	17472.0
70.10	1308.0
72.00	953.0
73.00	8191.0
74.10	30496.0
75.10	84344.0
76.10	7509.0
77.00	828.0
78.10	594.0
79.00	6639.0
80.00	1856.0
81.00	6457.0
81.90	1374.0
82.90	144.0
85.90	235.0
87.00	5254.0
88.00	5835.0
88.70	184.0
91.00	700.0
92.00	5434.0
93.00	7447.0
94.00	21800.0
95.10	164736.0
96.00	10863.0
97.00	298.0
103.90	871.0
105.00	246.0
105.90	924.0
106.80	240.0
109.70	148.0
110.80	227.0
111.90	172.0
112.90	176.0
114.90	205.0
115.90	598.0
116.90	1455.0
117.90	757.0
118.90	1225.0
123.90	106.0
127.90	624.0
128.90	353.0
129.80	785.0
130.80	287.0
134.90	378.0
137.00	363.0
140.10	206.0
141.00	2407.0
142.00	300.0
143.00	2632.0
144.00	173.0
144.90	499.0
145.90	279.0
146.90	126.0
147.90	347.0
148.60	113.0
149.10	158.0
149.90	229.0
151.80	141.0
153.00	152.0
153.90	129.0
154.90	519.0
157.00	338.0
158.80	199.0
160.70	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

161.10	175.0
170.80	221.0
172.00	1178.0
173.20	2267.0
174.00	153152.0
175.00	11738.0
176.00	147072.0
177.00	9978.0
178.00	244.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
36.00	1442.0
37.10	7008.0
38.10	6134.0
39.10	2407.0
40.00	2714.0
43.00	138.0
44.10	918.0
45.00	1363.0
46.00	160.0
47.00	1776.0
48.00	1103.0
49.00	6306.0
50.10	27776.0
51.10	8702.0
52.00	312.0
55.00	422.0
56.00	2422.0
57.10	4111.0
58.30	220.0
60.00	1506.0
61.10	7941.0
62.10	7508.0
63.10	5729.0
64.00	641.0
65.00	774.0
65.90	106.0
67.10	494.0
68.00	16000.0
69.00	16888.0
70.00	1131.0
72.00	974.0
73.00	7935.0
74.10	28888.0
75.10	81072.0
76.00	7331.0
77.00	781.0
77.90	489.0
79.00	6330.0
80.00	1764.0
81.00	6169.0
81.90	1444.0
82.90	142.0
85.90	236.0
87.00	5256.0
88.00	5615.0
91.00	696.0
92.00	5242.0
93.00	7233.0
94.00	21040.0
95.10	159616.0
96.10	9978.0
97.00	234.0
102.90	101.0
103.90	932.0
105.00	244.0
105.90	887.0
106.90	173.0
109.80	143.0
110.80	248.0
111.80	143.0
113.00	180.0
114.90	195.0
116.00	577.0
116.90	1404.0
118.00	675.0
118.90	1243.0
127.90	579.0
128.90	364.0
129.80	748.0
130.80	303.0
134.90	366.0
137.00	362.0
140.00	180.0
141.00	2459.0
142.10	336.0
143.00	2750.0
144.00	165.0
144.90	441.0
145.90	287.0
146.90	134.0
147.90	342.0
149.10	181.0
150.00	205.0
151.80	102.0
153.00	168.0
153.80	164.0
154.90	445.0
157.00	358.0
158.80	207.0
160.70	204.0
161.00	185.0
170.20	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

172.00	1015.0
174.00	150848.0
175.00	11289.0
176.00	145728.0
177.00	9582.0
177.90	249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257