
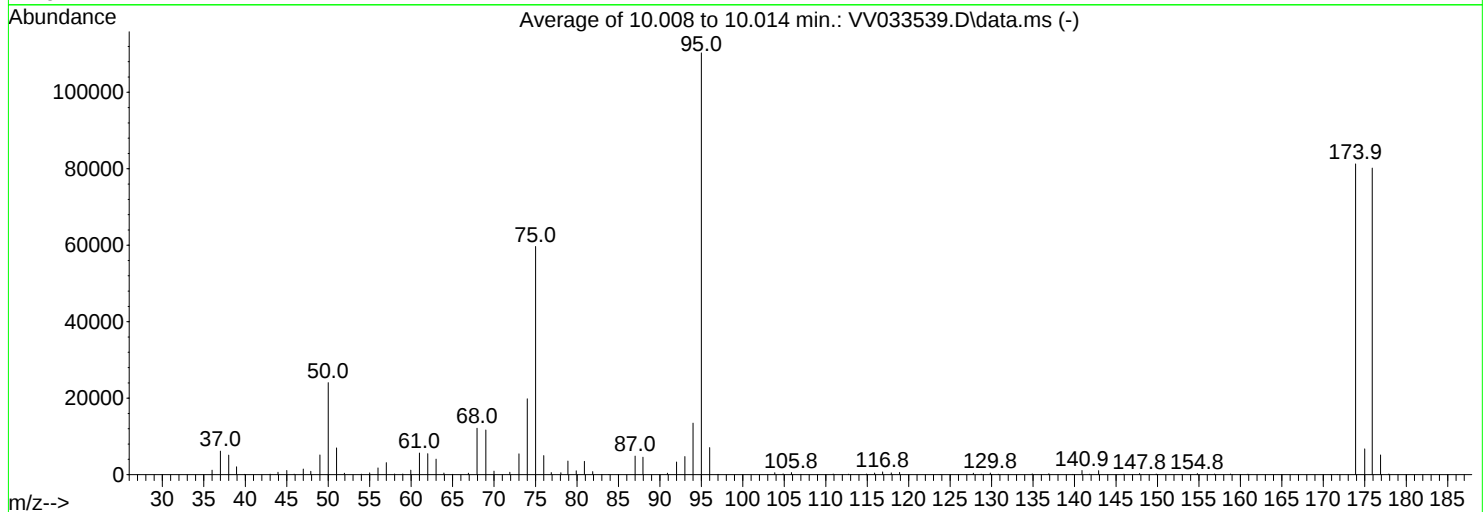


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122823\
Data File : VV033539.D
Acq On : 28 Dec 2023 08:26
Operator : SY/MD
Sample : BFB235
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB235

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 29 04:10:53 2023

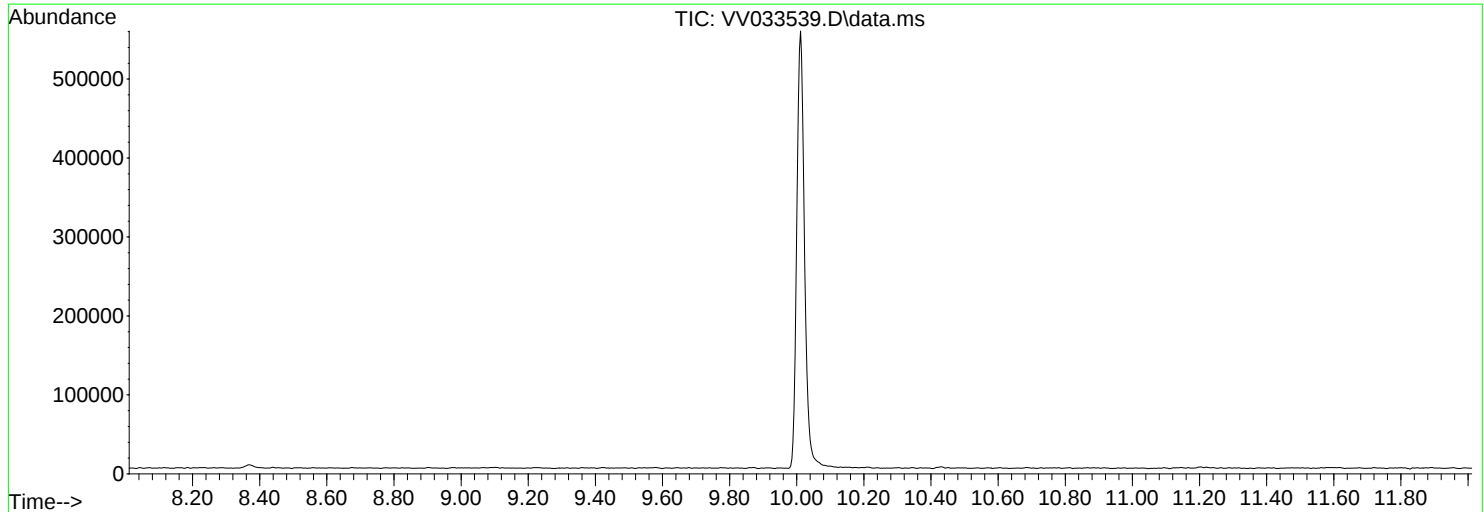

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	24056	PASS
75	95	30	80	54.1	59691	PASS
95	95	100	100	100.0	110320	PASS
96	95	5	9	6.4	7082	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.7	81253	PASS
175	174	5	9	8.3	6733	PASS
176	174	95	105	98.7	80173	PASS
177	176	5	10	6.4	5151	PASS

m/z	Abundance
38.90	198.0
40.00	236.0
41.00	690.0
41.90	240.0
43.00	624.0
43.90	768.0
53.00	119.0
55.00	498.0
56.00	258.0
57.10	624.0
58.00	132.0
66.80	181.0
67.90	116.0
69.00	336.0
70.10	161.0
71.00	317.0
76.90	173.0
80.90	255.0
82.00	120.0
83.10	210.0
83.80	109.0
85.10	195.0
91.00	107.0
95.10	144.0
96.10	134.0
97.10	237.0
98.00	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	1120.0
37.00	6319.0
38.00	5302.0
39.00	2301.0
39.90	315.0
41.00	630.0
42.00	201.0
43.00	696.0
44.00	1363.0
45.00	1121.0
45.90	103.0
47.10	1550.0
47.90	883.0
49.00	5199.0
50.00	24216.0
51.00	7114.0
52.00	352.0
54.00	117.0
55.00	941.0
56.00	2029.0
57.00	3745.0
58.00	281.0
59.00	152.0
59.90	1230.0
61.00	5693.0
62.00	5574.0
63.00	3980.0
63.90	463.0
67.00	606.0
68.00	12487.0
69.00	12186.0
70.00	1075.0
70.90	320.0
71.90	637.0
73.00	5568.0
74.00	19816.0
75.00	59720.0
76.00	4997.0
76.90	752.0
78.00	522.0
78.90	3665.0
79.90	968.0
80.90	3634.0
81.90	882.0
83.00	277.0
83.90	102.0
85.00	216.0
87.00	4647.0
88.00	4439.0
90.90	479.0
92.00	3393.0
93.00	4580.0
94.00	13455.0
95.00	109568.0
96.00	7298.0
97.00	341.0
97.90	116.0
103.80	525.0
104.80	208.0
105.90	517.0
110.90	196.0
112.80	109.0
114.90	178.0
115.90	435.0
116.90	724.0
117.90	454.0
118.90	585.0
123.80	118.0
127.80	362.0
128.80	155.0
129.90	423.0
130.80	155.0
134.90	217.0
136.90	234.0
139.80	118.0
140.90	1040.0
141.80	128.0
142.90	1095.0
146.00	127.0
147.90	292.0
149.80	163.0
152.90	104.0
154.80	297.0
156.90	180.0
158.80	165.0
160.90	112.0
173.90	78192.0
175.00	6658.0
175.90	77640.0
176.90	4970.0
177.90	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	1218.0
37.00	6401.0
38.00	5208.0
39.00	2303.0
39.90	351.0
40.90	646.0
42.00	207.0
43.00	739.0
44.00	1454.0
45.00	1124.0
45.90	125.0
47.00	1501.0
47.90	967.0
49.00	5347.0
50.00	24872.0
51.00	7177.0
52.00	372.0
54.00	127.0
55.00	995.0
56.00	2102.0
57.00	3874.0
58.00	304.0
59.00	170.0
60.00	1240.0
61.00	5884.0
62.00	5641.0
63.00	4164.0
63.90	439.0
65.00	115.0
67.00	569.0
68.00	12586.0
69.00	12390.0
70.00	1136.0
71.00	309.0
71.90	639.0
73.00	5648.0
74.00	20408.0
75.00	61696.0
76.00	5199.0
76.90	745.0
78.10	552.0
78.90	3684.0
79.90	1041.0
80.90	3883.0
81.90	926.0
83.00	255.0
84.00	146.0
85.00	274.0
87.00	5020.0
87.90	4738.0
90.90	513.0
92.00	3386.0
93.00	4902.0
94.00	14029.0
95.00	114296.0
96.00	7399.0
97.00	314.0
97.90	113.0
103.80	524.0
104.80	217.0
105.80	565.0
107.00	111.0
110.90	179.0
112.80	122.0
114.90	160.0
115.90	419.0
116.90	742.0
117.90	442.0
118.90	628.0
127.80	388.0
128.80	142.0
129.80	411.0
130.80	140.0
134.90	232.0
136.90	253.0
139.80	125.0
140.90	1099.0
141.80	123.0
142.90	1074.0
146.00	149.0
147.80	299.0
149.80	167.0
154.80	310.0
156.90	181.0
158.80	196.0
160.90	137.0
170.90	108.0
171.70	177.0
173.90	83968.0
175.00	6935.0
175.90	82696.0
176.90	5347.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

177.90

193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	1164.0
37.00	5790.0
38.00	4755.0
39.00	2097.0
39.90	351.0
40.90	654.0
42.00	203.0
43.00	777.0
44.00	1388.0
45.00	1024.0
45.90	121.0
46.90	1330.0
47.90	848.0
49.00	4944.0
50.00	23080.0
51.00	6650.0
51.90	376.0
53.00	106.0
54.00	130.0
55.00	987.0
56.00	1956.0
57.00	3624.0
58.00	292.0
59.00	150.0
60.00	1115.0
61.00	5363.0
62.00	5277.0
63.00	3988.0
64.00	408.0
65.00	105.0
66.90	494.0
68.00	11640.0
69.00	11427.0
70.00	1036.0
71.00	320.0
71.90	648.0
73.00	5159.0
74.00	19344.0
75.00	57656.0
76.00	4776.0
76.90	693.0
78.10	492.0
78.90	3368.0
79.90	1001.0
80.90	3680.0
81.90	895.0
83.00	275.0
84.00	197.0
85.00	276.0
87.00	4869.0
87.90	4507.0
90.90	471.0
92.00	3195.0
93.00	4683.0
94.00	13003.0
95.00	107528.0
96.00	6950.0
97.00	276.0
98.00	113.0
103.90	503.0
104.90	196.0
105.90	579.0
107.00	105.0
110.00	106.0
110.90	151.0
112.60	120.0
113.00	124.0
114.90	119.0
115.90	369.0
116.80	675.0
117.90	444.0
118.90	588.0
127.80	392.0
128.70	120.0
129.80	366.0
130.80	111.0
134.90	229.0
136.90	231.0
140.90	1081.0
141.80	118.0
142.90	1000.0
145.90	163.0
147.80	247.0
149.90	139.0
154.80	275.0
156.90	167.0
158.80	185.0
160.90	146.0
173.90	81600.0
175.00	6607.0
175.90	80184.0
176.90	5136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

177.90

185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235