


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV122920\
 Data File : VV019854.D
 Acq On : 29 Dec 2020 09:45
 Operator : SY/MD
 Sample : BFB75
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB75

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR122920WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Dec 30 04:48:15 2020

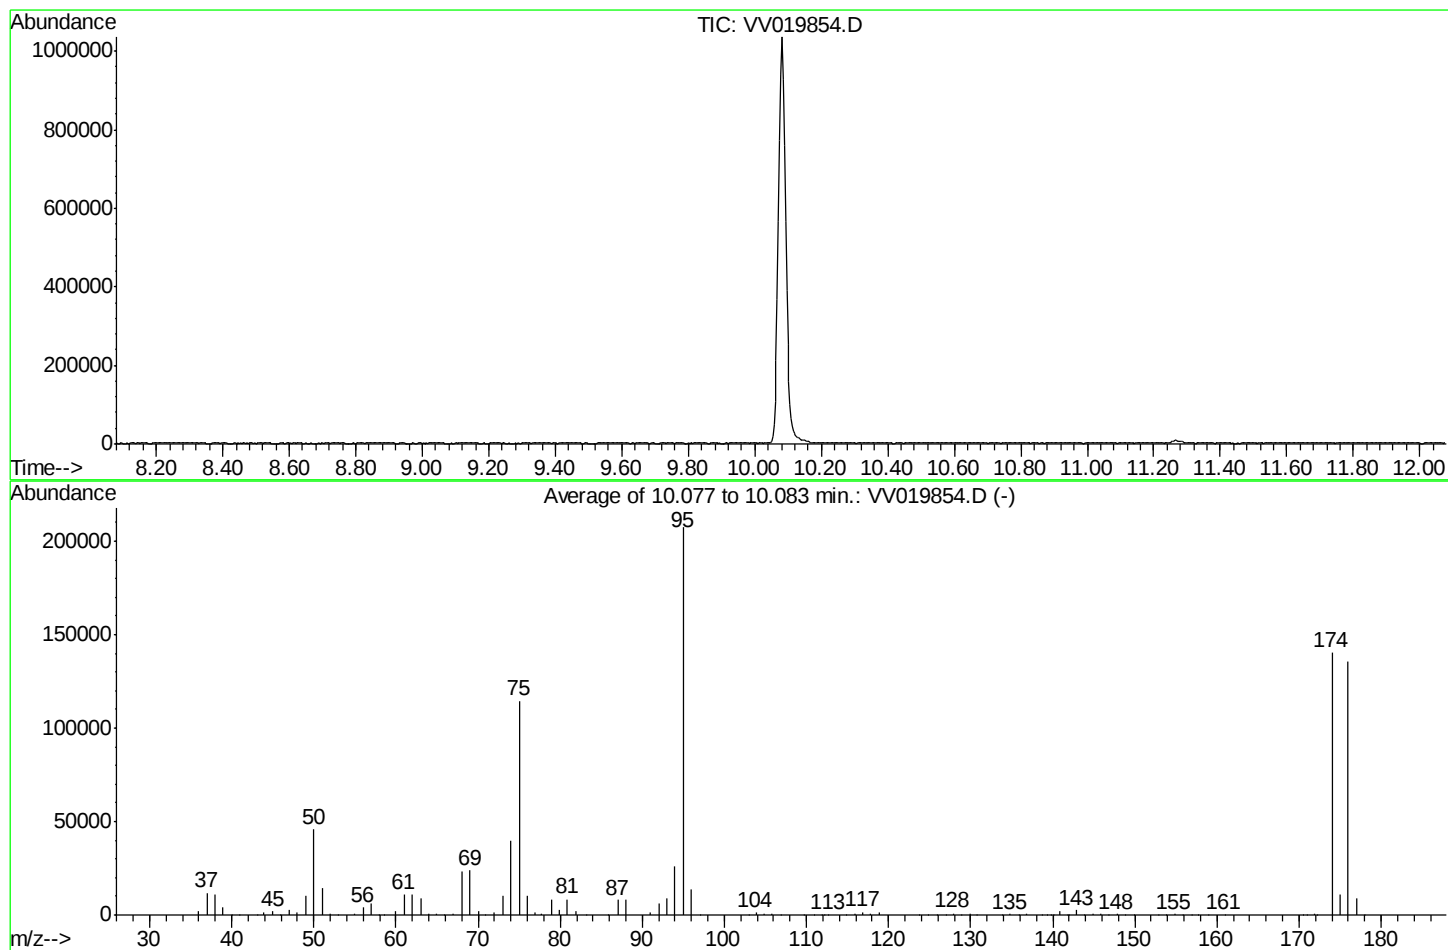

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2782

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	45690	PASS
75	95	30	80	55.2	114554	PASS
95	95	100	100	100.0	207488	PASS
96	95	5	9	6.5	13401	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.6	140181	PASS
175	174	5	9	8.1	11320	PASS
176	174	95	105	96.7	135624	PASS
177	176	5	10	6.6	9011	PASS

m/z	Abundance
36.00	2116.0
37.00	11561.0
38.00	10779.0
39.00	4151.0
39.90	478.0
40.90	153.0
42.00	106.0
43.20	233.0
44.00	2263.0
45.00	1814.0
45.90	353.0
47.00	2538.0
47.90	1312.0
49.00	9448.0
50.00	44176.0
51.00	13936.0
52.00	604.0
52.90	170.0
54.90	568.0
56.00	3630.0
57.00	5877.0
57.90	392.0
58.60	134.0
60.00	2141.0
61.00	10359.0
62.00	10066.0
63.00	8445.0
64.00	936.0
65.00	770.0
67.00	710.0
68.00	22208.0
69.00	22544.0
70.00	1817.0
70.90	119.0
72.00	1432.0
73.00	9191.0
74.00	37432.0
75.00	108704.0
76.00	9487.0
76.90	1209.0
77.70	690.0
78.90	7933.0
79.90	2250.0
80.90	7863.0
81.90	1806.0
83.10	219.0
85.90	272.0
87.00	7885.0
87.90	7728.0
91.00	920.0
92.00	5560.0
93.00	8763.0
94.00	24328.0
95.00	196032.0
96.00	12816.0
97.00	344.0
103.90	1067.0
104.80	413.0
105.80	992.0
106.80	299.0
109.70	219.0
110.90	179.0
111.90	194.0
112.70	263.0
114.90	257.0
115.80	662.0
116.90	1453.0
117.80	793.0
118.80	901.0
123.80	151.0
125.90	104.0
127.90	656.0
128.80	325.0
129.90	653.0
130.80	328.0
133.90	104.0
134.90	405.0
136.80	384.0
140.00	134.0
140.90	1823.0
141.80	296.0
142.90	2279.0
143.80	129.0
144.90	396.0
145.90	349.0
146.90	144.0
147.80	453.0
148.80	165.0
149.80	276.0
152.80	220.0
153.80	132.0
154.80	442.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

156.90	263.0
159.00	185.0
160.90	321.0
170.80	146.0
171.90	765.0
172.20	654.0
174.00	128640.0
175.00	10897.0
176.00	123800.0
177.00	8490.0
178.00	301.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	2198.0
37.00	12062.0
38.00	11265.0
39.00	4276.0
39.90	457.0
40.90	151.0
43.20	285.0
44.00	2453.0
45.00	2003.0
45.90	320.0
47.00	2960.0
47.90	1489.0
49.00	10421.0
50.00	47280.0
51.00	15199.0
52.00	635.0
53.00	136.0
54.90	653.0
56.00	4133.0
57.00	6542.0
57.90	396.0
60.00	2448.0
61.00	11108.0
62.00	11168.0
63.00	9123.0
64.00	971.0
65.00	805.0
67.00	769.0
68.00	24528.0
69.00	24432.0
70.00	1969.0
70.90	130.0
72.00	1509.0
73.00	10690.0
74.00	40880.0
75.00	118256.0
76.00	10381.0
76.90	1236.0
77.80	793.0
78.90	8483.0
79.90	2521.0
80.90	8473.0
81.90	1921.0
83.10	257.0
85.80	263.0
87.00	8390.0
88.00	8163.0
90.90	1134.0
92.00	6322.0
93.00	9478.0
94.00	27064.0
95.00	213824.0
96.00	13799.0
97.00	324.0
102.90	127.0
103.90	1255.0
104.90	429.0
105.90	1031.0
106.80	305.0
109.80	239.0
111.00	211.0
112.10	168.0
112.70	244.0
114.80	292.0
115.90	835.0
116.90	1610.0
117.80	848.0
118.80	1099.0
123.70	160.0
125.90	153.0
127.00	120.0
127.90	823.0
128.80	354.0
129.90	811.0
130.80	334.0
133.90	149.0
134.90	438.0
135.90	115.0
136.80	410.0
138.70	140.0
139.70	126.0
140.00	125.0
140.90	2005.0
141.70	300.0
142.90	2550.0
143.90	159.0
144.90	420.0
145.90	402.0
146.80	153.0
147.80	486.0
148.80	138.0
149.80	236.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

152.80	219.0
153.80	119.0
154.80	546.0
156.90	275.0
157.70	113.0
159.00	200.0
160.90	377.0
170.50	109.0
170.90	165.0
171.90	932.0
174.00	144832.0
175.00	11687.0
176.00	140352.0
177.00	9307.0
177.90	345.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	2071.0
37.00	11711.0
38.00	10706.0
39.00	4030.0
39.90	418.0
40.90	144.0
43.20	285.0
44.00	2457.0
45.00	1957.0
46.00	323.0
47.00	3186.0
48.00	1526.0
49.00	10334.0
50.00	45616.0
51.00	14768.0
52.00	673.0
55.00	666.0
56.00	4118.0
57.00	6611.0
58.00	270.0
60.00	2439.0
61.00	10952.0
62.00	11007.0
63.00	8849.0
64.00	923.0
65.00	775.0
65.90	128.0
66.90	731.0
68.00	24056.0
69.00	24152.0
70.00	1976.0
72.00	1430.0
73.00	10986.0
74.00	40032.0
75.00	116704.0
76.00	10526.0
77.00	1276.0
77.80	808.0
78.90	7946.0
79.90	2535.0
80.90	8536.0
81.90	1881.0
83.10	224.0
85.80	271.0
87.00	8313.0
88.00	7889.0
90.90	1234.0
92.00	6570.0
93.00	9563.0
94.00	26872.0
95.00	212608.0
96.00	13589.0
97.00	324.0
102.90	168.0
103.90	1250.0
104.90	368.0
105.90	974.0
106.90	291.0
109.80	214.0
111.00	253.0
112.10	168.0
112.70	198.0
114.80	300.0
115.90	973.0
116.90	1574.0
117.90	783.0
118.80	1169.0
123.70	140.0
124.80	111.0
125.90	157.0
127.00	131.0
127.90	853.0
128.90	374.0
129.90	852.0
130.80	341.0
133.90	152.0
134.80	410.0
135.90	124.0
136.90	436.0
138.70	179.0
139.30	116.0
140.00	135.0
140.90	2071.0
141.80	226.0
142.00	218.0
142.90	2666.0
143.90	142.0
144.80	371.0
145.80	410.0
146.80	174.0
147.80	480.0
148.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

149.90	185.0
152.90	170.0
153.70	107.0
154.90	518.0
155.80	134.0
156.90	259.0
157.70	158.0
158.80	241.0
160.90	336.0
171.00	143.0
171.90	979.0
174.00	147072.0
175.00	11376.0
176.00	142720.0
177.00	9236.0
177.90	328.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	116.0
36.90	124.0
37.70	110.0
38.90	131.0
39.90	357.0
41.90	114.0
43.10	142.0
43.90	1034.0
45.00	155.0
52.00	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75