

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV123019\
 Data File : VV014225.D
 Acq On : 30 Dec 2019 17:56
 Operator : SY/MD
 Sample : K6459-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0BP8

Quant Time: Dec 31 06:45:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 31 06:00:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	824322	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	755059	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	351237	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	229014	5.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.60%
7) Chloroethane-d5	1.59	69	205457	6.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	127.80%
11) 1,1-Dichloroethene-d2	2.13	63	297959	4.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.00%
20) 2-Butanone-d5	3.92	46	659092	68.73	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	137.46%#
24) Chloroform-d	4.40	84	455398	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.08	65	266669	5.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.20%
32) Benzene-d6	5.10	84	1068264	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
36) 1,2-Dichloropropane-d6	6.12	67	341366	5.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.40%
41) Toluene-d8	7.36	98	982166	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.00%
43) trans-1,3-Dichloropropene-	7.66	79	141516	5.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.40%
46) 2-Hexanone-d5	8.13	63	575109	54.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.56%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	238864	5.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	323762	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%


Target Compounds					Ovalue
25) Chloroform	4.42	83	63316	0.592 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV123019\
Data File : VV014225.D
Acq On : 30 Dec 2019 17:56
Operator : SY/MD
Sample : K6459-09
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0BP8

Quant Time: Dec 31 06:45:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 31 06:00:54 2019
Response via : Initial Calibration

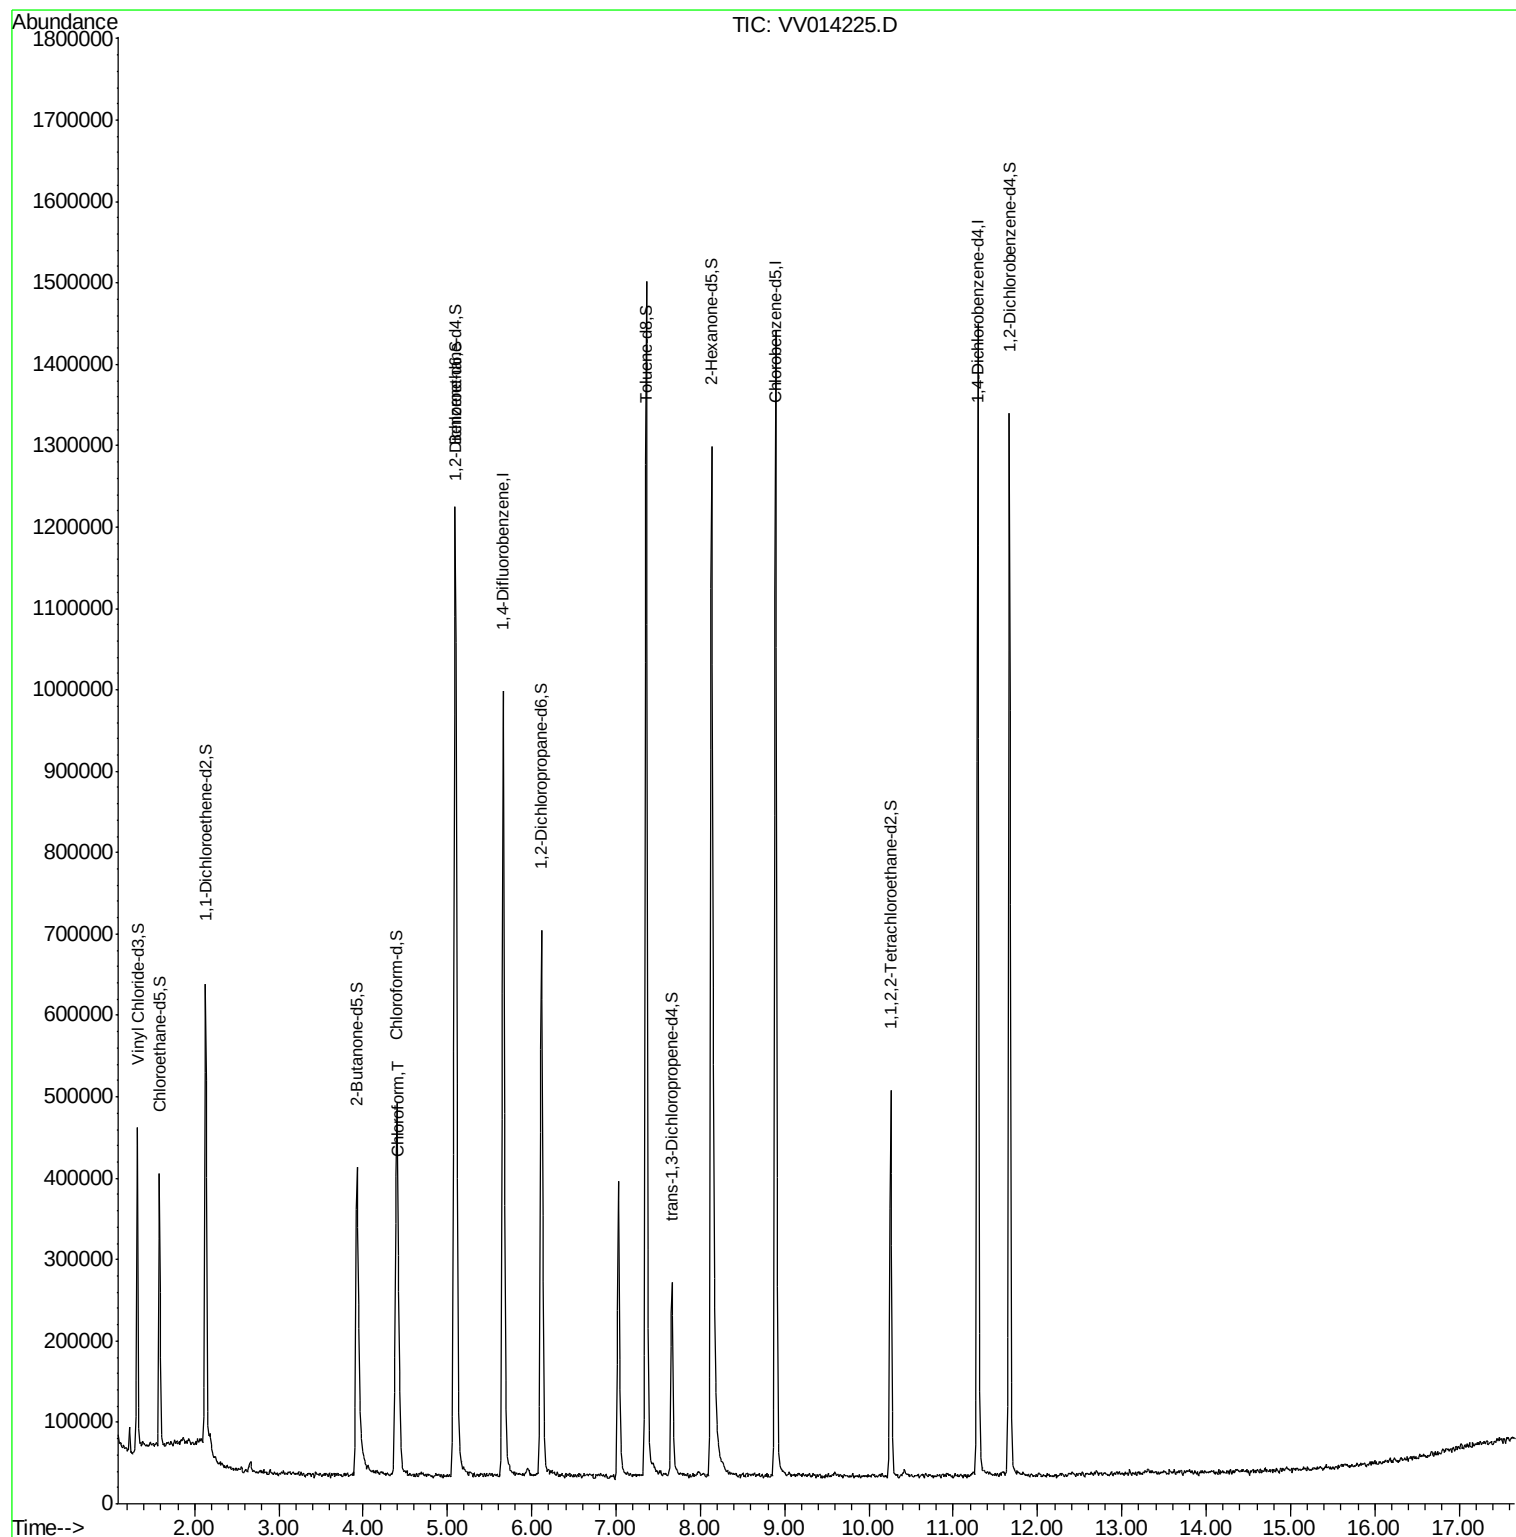

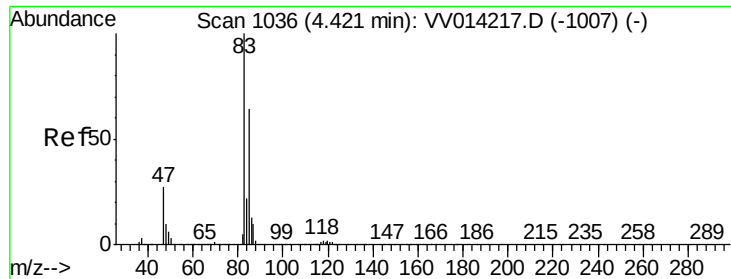

#25
Chloroform
Concen: 0.592 ug/L
RT: 4.42 min Scan# 1037
Delta R.T. 0.00 min
Lab File: VV014225.D
Acq: 30 Dec 2019 17:56

Instrument :
MSVOA_V
ClientSampleId :
H0BP8

Tot Ion: 83 Resp: 63316
Ion Ratio Lower Upper
83 100
85 61.3 46.2 85.8

