


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV123019\
 Data File : VV014216.D
 Acq On : 30 Dec 2019 12:36
 Operator : SY/MD
 Sample : BFB48
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB48

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jan 01 03:03:23 2020

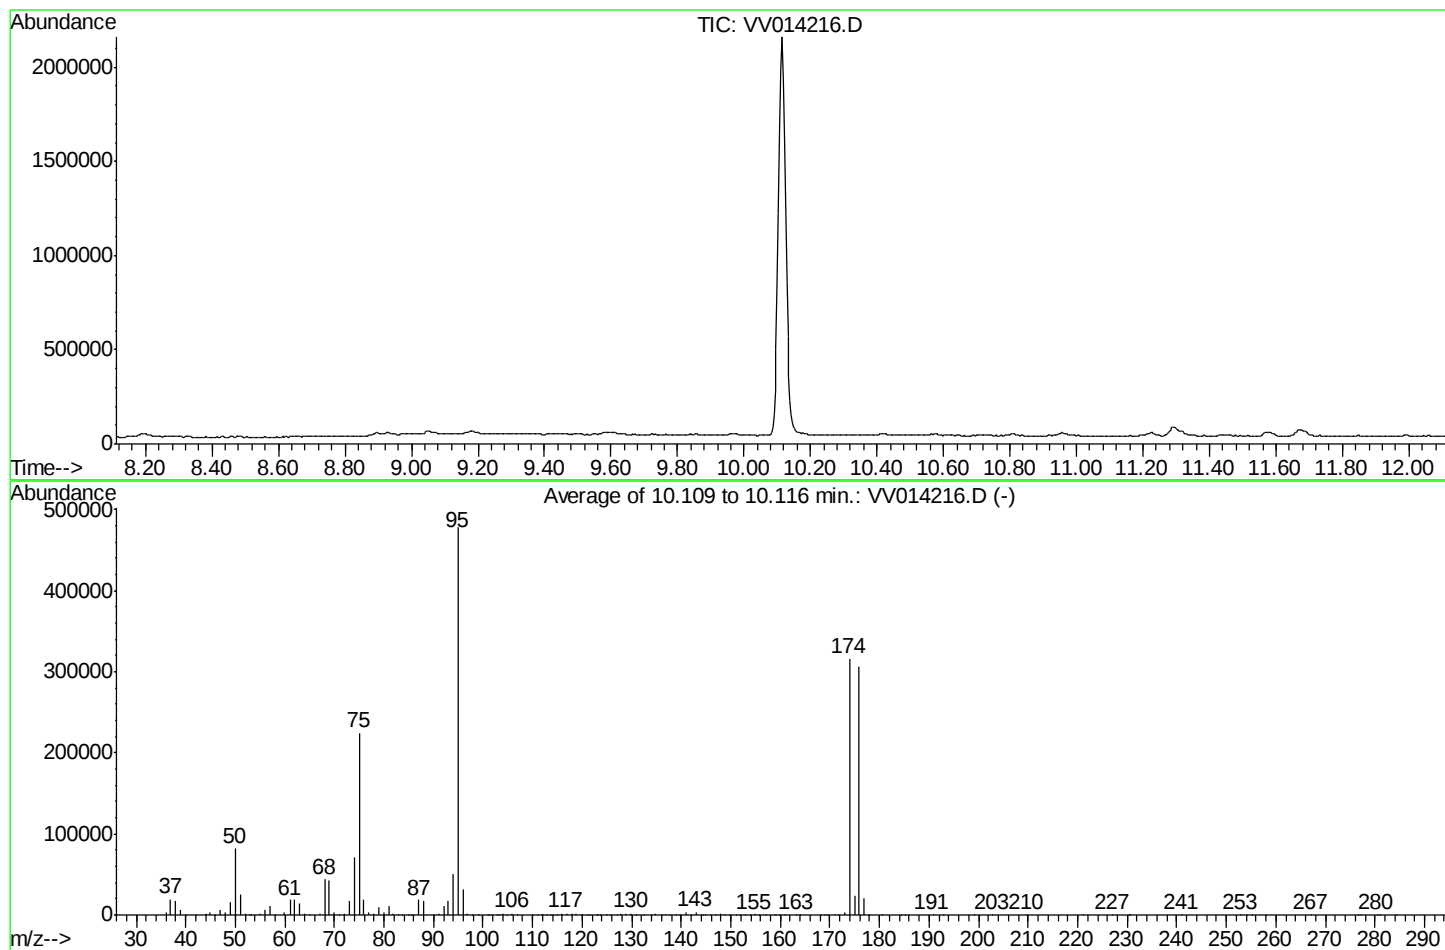

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	81500	PASS
75	95	30	80	46.9	224234	PASS
95	95	100	100	100.0	477904	PASS
96	95	5	9	6.7	31791	PASS
173	174	0.00	2	1.1	3540	PASS
174	95	50	120	66.2	316160	PASS
175	174	5	9	7.6	24170	PASS
176	174	95	101	97.0	306645	PASS
177	176	5	9	6.5	19784	PASS

m/z	Abundance
36.00	10411.0
37.00	19760.0
38.00	18216.0
39.00	7212.0
39.90	1782.0
41.00	1406.0
42.00	846.0
42.90	1347.0
44.00	4375.0
45.00	3162.0
46.00	317.0
47.00	5115.0
48.00	2654.0
49.00	16392.0
50.00	79520.0
51.00	25352.0
52.00	1076.0
53.00	455.0
54.20	442.0
55.00	2473.0
56.00	6004.0
57.00	11248.0
58.00	542.0
58.90	406.0
60.00	3888.0
61.00	18632.0
62.00	18448.0
63.00	14063.0
63.90	1060.0
65.00	275.0
67.00	1641.0
68.00	41792.0
69.00	41632.0
70.00	3598.0
71.00	976.0
71.90	2081.0
73.00	17144.0
74.00	68320.0
75.00	211584.0
76.00	18840.0
77.00	3179.0
77.90	1708.0
78.90	9795.0
80.00	2590.0
80.90	10569.0
81.90	2566.0
82.90	849.0
84.10	223.0
84.90	459.0
85.30	360.0
86.10	443.0
87.00	17832.0
88.00	17480.0
91.00	1737.0
92.00	11434.0
93.00	16616.0
94.00	48088.0
95.00	448256.0
96.00	32136.0
96.90	1226.0
97.80	544.0
99.30	224.0
101.10	125.0
101.60	123.0
102.70	138.0
103.20	249.0
103.90	1601.0
104.90	628.0
105.90	2056.0
106.80	606.0
107.80	109.0
109.90	293.0
110.90	487.0
111.70	340.0
113.00	591.0
114.90	584.0
115.90	1364.0
116.90	2301.0
118.00	1501.0
118.90	1934.0
119.80	123.0
121.80	192.0
122.80	249.0
123.80	408.0
125.80	212.0
127.00	341.0
127.80	1268.0
128.80	1055.0
129.90	1834.0
130.90	817.0
133.00	155.0
133.80	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

134.80	873.0
136.00	297.0
136.70	757.0
137.60	177.0
138.80	250.0
139.70	466.0
140.90	3483.0
141.90	552.0
142.90	4007.0
143.90	453.0
144.90	476.0
145.80	558.0
146.90	314.0
147.90	1073.0
148.80	411.0
149.80	358.0
150.80	124.0
151.70	236.0
152.80	310.0
153.90	268.0
154.90	1032.0
155.90	188.0
157.00	684.0
158.80	407.0
159.70	103.0
160.80	276.0
163.20	181.0
168.80	118.0
169.30	200.0
170.00	151.0
171.00	484.0
173.00	3447.0
173.90	296064.0
175.00	22984.0
175.90	284160.0
176.90	18624.0
177.90	503.0
180.50	132.0
184.40	124.0
185.20	114.0
199.00	110.0
209.80	163.0
220.90	138.0
230.60	131.0
239.10	127.0
241.00	148.0
252.90	129.0
257.90	103.0
267.10	152.0
281.00	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	10524.0
37.00	20768.0
38.00	19896.0
39.00	7913.0
40.00	1834.0
41.00	1409.0
42.10	648.0
42.90	1572.0
43.90	4406.0
45.00	3128.0
46.00	258.0
47.00	6142.0
48.00	2994.0
49.00	16816.0
50.00	84648.0
51.00	27064.0
52.00	1307.0
52.80	336.0
54.20	439.0
55.00	2465.0
56.00	6614.0
57.00	12151.0
57.90	580.0
58.90	303.0
60.00	4166.0
61.00	19080.0
62.00	19240.0
63.00	15150.0
63.90	1249.0
65.10	286.0
67.00	1566.0
68.00	44624.0
69.00	44264.0
70.00	3463.0
71.10	1162.0
71.90	2416.0
73.00	18584.0
74.00	73344.0
75.00	232320.0
76.00	20376.0
77.00	2981.0
78.00	1841.0
78.90	10650.0
80.00	2853.0
80.90	11629.0
81.90	2648.0
83.00	806.0
83.70	224.0
84.20	296.0
84.90	577.0
86.00	664.0
87.00	19848.0
88.00	18376.0
91.00	1959.0
92.00	12027.0
93.00	18584.0
94.00	52008.0
95.00	494464.0
96.00	33504.0
96.90	1249.0
97.80	611.0
99.20	309.0
99.90	106.0
101.20	124.0
101.70	101.0
102.70	167.0
103.90	1801.0
104.90	720.0
105.90	2068.0
106.80	637.0
107.80	114.0
109.10	185.0
109.90	322.0
110.80	599.0
111.80	337.0
112.90	617.0
113.50	112.0
114.90	566.0
115.90	1449.0
116.90	2415.0
118.00	1670.0
118.90	2256.0
120.10	124.0
121.00	103.0
121.80	210.0
122.70	207.0
123.10	183.0
123.70	457.0
125.10	251.0
125.70	272.0
127.10	329.0
127.80	1434.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

128.80	947.0
129.90	2082.0
130.90	855.0
133.10	145.0
133.90	197.0
134.80	1067.0
136.00	356.0
136.80	830.0
137.50	156.0
138.80	325.0
139.80	462.0
140.90	4070.0
141.90	731.0
142.90	4140.0
143.90	370.0
144.40	277.0
145.00	467.0
145.80	734.0
146.90	231.0
147.90	1136.0
148.80	446.0
149.90	478.0
150.90	159.0
151.80	245.0
152.80	291.0
153.80	231.0
154.90	1160.0
155.90	221.0
157.00	662.0
158.80	413.0
159.70	156.0
160.80	336.0
163.20	105.0
164.00	127.0
168.00	110.0
168.80	186.0
169.30	188.0
169.90	174.0
170.90	510.0
173.00	3573.0
173.90	325184.0
175.00	24864.0
175.90	315072.0
177.00	20384.0
177.90	601.0
185.20	101.0
190.70	105.0
199.00	139.0
202.80	120.0
207.10	157.0
209.70	124.0
227.00	103.0
230.30	103.0
230.70	115.0
239.00	167.0
252.90	146.0
267.10	136.0
277.20	114.0
280.40	141.0
280.90	156.0
284.40	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	10635.0
37.00	20336.0
38.00	19768.0
39.00	7632.0
40.00	1903.0
41.00	1402.0
42.10	551.0
42.90	1552.0
43.90	4164.0
45.00	3017.0
46.00	275.0
47.00	6384.0
48.00	3001.0
49.00	16150.0
50.00	81200.0
51.00	26384.0
52.00	1352.0
52.70	300.0
53.20	252.0
54.30	339.0
55.00	2479.0
56.00	6676.0
57.00	11592.0
57.90	665.0
60.00	3961.0
61.00	18224.0
62.00	18408.0
63.00	14337.0
63.90	1305.0
65.10	261.0
67.00	1150.0
68.00	44008.0
69.00	43712.0
70.00	3194.0
71.10	1215.0
71.90	2517.0
73.00	18224.0
74.00	72168.0
75.00	229376.0
76.00	19704.0
77.00	2430.0
78.00	1755.0
78.90	10390.0
80.00	2913.0
80.90	11556.0
81.90	2539.0
83.00	808.0
84.20	434.0
84.90	576.0
86.00	732.0
87.00	19120.0
88.00	18248.0
90.10	159.0
91.00	2049.0
92.00	11830.0
93.00	18744.0
94.00	51904.0
95.00	491776.0
96.00	31568.0
97.00	1219.0
97.80	624.0
99.20	345.0
99.90	154.0
100.90	116.0
102.80	211.0
103.10	219.0
103.90	2066.0
104.90	760.0
105.90	1827.0
106.90	641.0
107.90	165.0
109.00	165.0
109.90	303.0
110.80	591.0
112.00	380.0
112.90	525.0
114.00	140.0
114.90	554.0
115.90	1361.0
116.90	2426.0
118.00	1547.0
118.90	2403.0
120.10	156.0
121.00	140.0
121.60	258.0
122.70	193.0
123.10	182.0
123.70	399.0
125.00	321.0
125.70	249.0
127.10	347.0
127.90	1472.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

128.70	806.0
128.80	800.0
129.90	1964.0
130.90	832.0
132.30	133.0
133.10	119.0
133.90	165.0
134.80	997.0
136.00	301.0
136.80	793.0
138.80	371.0
139.80	409.0
140.90	4137.0
141.90	685.0
143.00	3816.0
143.90	267.0
145.00	477.0
145.70	790.0
147.90	1030.0
148.80	495.0
149.90	585.0
151.00	146.0
151.90	319.0
152.90	328.0
153.80	234.0
154.90	1269.0
155.90	179.0
156.90	667.0
159.00	470.0
159.80	173.0
160.90	436.0
167.90	140.0
168.80	212.0
169.30	171.0
170.90	465.0
171.80	595.0
173.00	3602.0
173.90	327232.0
175.00	24664.0
175.90	320704.0
177.00	20344.0
177.90	620.0
190.70	143.0
192.90	103.0
202.70	177.0
207.10	172.0
227.10	161.0
239.00	172.0
252.90	118.0
254.20	104.0
255.00	107.0
267.10	110.0
276.50	107.0
277.20	134.0
280.40	199.0
284.40	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	7581.0
36.90	709.0
37.90	2605.0
39.10	981.0
39.90	1763.0
41.00	1505.0
42.00	668.0
43.00	1667.0
44.00	2251.0
44.90	277.0
46.10	263.0
47.50	176.0
48.00	152.0
49.20	218.0
50.10	289.0
51.10	212.0
52.20	136.0
52.90	336.0
53.50	416.0
54.20	411.0
55.00	1297.0
56.10	727.0
57.00	1083.0
57.90	220.0
58.70	193.0
59.00	171.0
59.90	456.0
61.20	195.0
62.60	157.0
64.10	169.0
64.70	207.0
65.20	201.0
66.20	223.0
67.00	460.0
68.40	219.0
69.10	888.0
70.10	580.0
71.00	504.0
71.80	133.0
73.20	210.0
73.90	182.0
74.90	192.0
75.90	128.0
76.60	242.0
77.10	171.0
77.90	171.0
79.00	274.0
79.70	146.0
80.90	490.0
81.90	507.0
82.90	503.0
84.10	472.0
85.00	420.0
87.00	148.0
88.20	163.0
89.10	114.0
91.00	447.0
92.20	146.0
93.10	332.0
94.00	147.0
94.90	261.0
95.80	611.0
96.80	281.0
97.30	296.0
98.10	523.0
98.70	223.0
99.20	172.0
99.90	103.0
102.70	110.0
104.40	103.0
105.10	229.0
105.80	150.0
106.20	104.0
107.80	135.0
109.20	241.0
110.20	244.0
111.00	386.0
112.40	237.0
112.80	186.0
114.90	286.0
116.80	166.0
118.70	154.0
122.00	115.0
124.00	163.0
125.10	168.0
125.80	174.0
127.10	165.0
129.00	220.0
129.90	154.0
132.90	171.0
136.00	129.0
136.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

139.40	108.0
140.80	140.0
144.10	135.0
145.90	156.0
147.30	264.0
150.10	205.0
151.90	187.0
153.10	129.0
154.00	213.0
154.90	158.0
155.70	118.0
156.80	158.0
158.30	112.0
165.00	157.0
170.00	127.0
178.40	127.0
180.00	112.0
187.70	118.0
195.90	127.0
196.70	158.0
207.10	177.0
225.70	118.0
227.50	129.0
236.10	146.0
239.00	181.0
243.20	140.0
251.60	113.0
252.50	119.0
282.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48