


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV123020\
 Data File : VV019870.D
 Acq On : 30 Dec 2020 09:17
 Operator : SY/MD
 Sample : BFB76
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB76

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR122920WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 31 02:03:35 2020

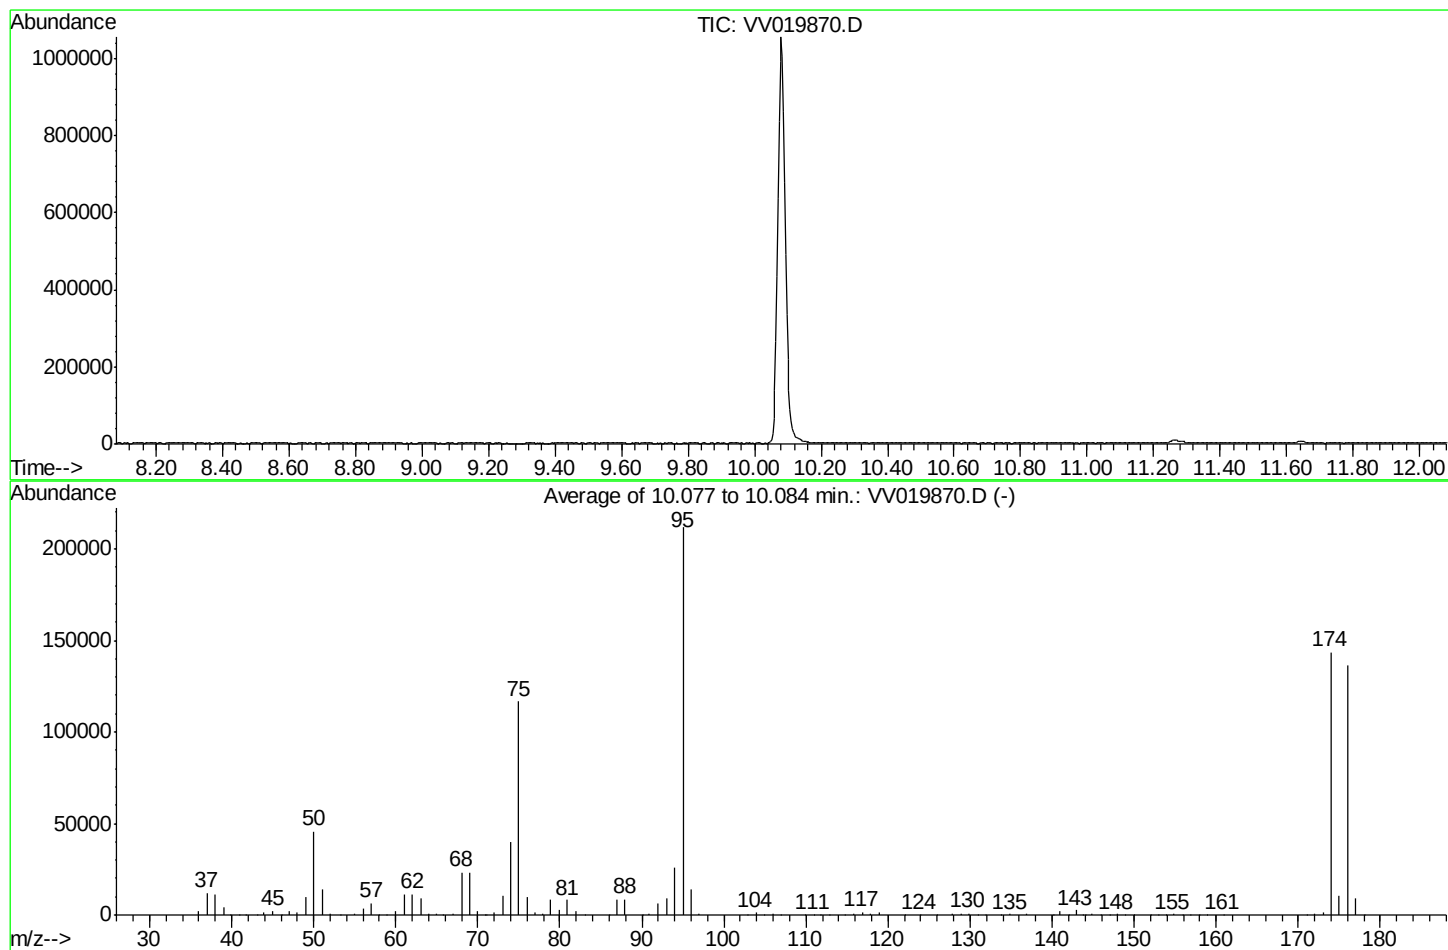

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2782

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	45730	PASS
75	95	30	80	55.1	116704	PASS
95	95	100	100	100.0	211818	PASS
96	95	5	9	6.6	14018	PASS
173	174	0.00	2	1.2	1725	PASS
174	95	50	120	67.7	143488	PASS
175	174	5	9	7.3	10425	PASS
176	174	95	105	95.1	136418	PASS
177	176	5	10	6.7	9114	PASS

m/z	Abundance
36.00	2244.0
37.00	12203.0
38.00	10817.0
39.00	4392.0
39.90	357.0
40.90	181.0
41.60	101.0
43.00	308.0
44.00	2050.0
45.00	2157.0
46.00	315.0
47.00	2315.0
48.00	1388.0
49.00	9964.0
50.00	45528.0
51.00	14237.0
52.00	585.0
53.20	162.0
55.00	680.0
56.00	3502.0
57.00	6652.0
57.90	348.0
58.90	130.0
60.00	2395.0
61.00	11215.0
62.00	10887.0
63.00	9070.0
64.00	957.0
65.00	730.0
65.70	153.0
67.00	603.0
68.00	23384.0
69.00	22232.0
70.00	2338.0
70.90	163.0
72.00	1078.0
73.00	10035.0
74.00	39232.0
75.00	114816.0
76.00	9896.0
76.90	1498.0
77.90	710.0
78.90	8413.0
80.00	2556.0
80.90	8096.0
81.90	1900.0
83.00	257.0
86.00	260.0
87.00	7962.0
88.00	8458.0
90.80	1027.0
92.00	6620.0
93.00	8676.0
94.00	25408.0
95.00	207424.0
96.00	14435.0
96.90	487.0
102.80	132.0
103.90	1073.0
105.00	344.0
106.00	1053.0
106.90	237.0
109.80	193.0
110.90	349.0
111.80	259.0
112.90	232.0
114.90	196.0
115.80	869.0
116.90	1477.0
117.90	938.0
118.90	1143.0
122.00	131.0
123.90	158.0
125.90	149.0
127.80	803.0
128.80	422.0
129.80	996.0
131.00	236.0
131.90	103.0
133.70	128.0
134.80	377.0
136.80	405.0
140.90	2096.0
142.00	368.0
142.90	2581.0
143.80	218.0
144.90	474.0
145.90	334.0
146.90	171.0
147.90	456.0
148.90	175.0
149.90	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

151.90	156.0
152.90	189.0
154.80	543.0
156.90	339.0
158.80	207.0
160.90	243.0
171.10	273.0
172.00	867.0
173.10	1780.0
174.00	136640.0
175.00	9973.0
176.00	130344.0
177.00	8766.0
178.00	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.00	2220.0
37.00	12452.0
38.00	11336.0
39.00	4475.0
39.90	400.0
40.90	242.0
41.60	106.0
43.10	294.0
44.00	2157.0
45.00	2235.0
46.00	363.0
47.10	2259.0
48.00	1544.0
49.00	10383.0
50.00	47440.0
51.00	14754.0
52.00	621.0
53.20	125.0
55.00	760.0
56.00	3826.0
57.00	6786.0
57.90	319.0
60.00	2383.0
61.00	11329.0
62.00	12063.0
63.00	9269.0
64.00	981.0
65.00	662.0
65.70	157.0
67.00	670.0
68.00	24144.0
69.00	23936.0
70.00	2463.0
70.90	150.0
72.00	1133.0
73.00	10716.0
74.00	41784.0
75.00	121008.0
76.00	10233.0
77.00	1508.0
77.90	697.0
78.90	8613.0
80.00	2643.0
80.90	8691.0
81.90	2028.0
83.00	247.0
86.00	249.0
87.00	8419.0
88.00	9027.0
90.90	983.0
92.00	6875.0
93.00	9279.0
94.00	27216.0
95.00	219456.0
96.00	14553.0
96.90	517.0
102.80	119.0
103.90	1174.0
105.00	348.0
105.90	1080.0
106.90	294.0
109.90	189.0
110.90	338.0
111.80	286.0
112.90	261.0
114.70	246.0
115.80	884.0
116.90	1505.0
117.90	903.0
118.90	1245.0
122.00	151.0
123.90	182.0
127.80	808.0
128.90	474.0
129.90	990.0
131.00	259.0
133.70	100.0
134.90	436.0
136.80	439.0
140.90	2385.0
142.00	357.0
142.90	2797.0
143.80	229.0
144.10	218.0
144.90	406.0
145.90	321.0
146.90	226.0
147.90	457.0
149.00	204.0
149.90	303.0
152.00	161.0
152.90	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

153.90	123.0
154.80	499.0
155.80	118.0
156.90	357.0
158.80	240.0
160.90	248.0
171.10	261.0
172.00	947.0
173.00	1778.0
174.00	149056.0
175.00	10893.0
176.00	141184.0
177.00	9495.0
178.10	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.00	1992.0
37.00	11483.0
38.00	10629.0
39.00	4116.0
39.90	408.0
40.90	242.0
41.70	101.0
43.00	235.0
44.00	2202.0
45.00	2216.0
46.00	415.0
47.00	2044.0
48.00	1495.0
49.00	9594.0
50.00	44224.0
51.00	13637.0
52.00	611.0
54.90	732.0
56.00	3672.0
57.00	6379.0
57.90	258.0
60.00	2098.0
61.00	10594.0
62.00	11712.0
63.00	8110.0
64.00	899.0
65.00	537.0
65.70	159.0
67.00	641.0
68.00	22568.0
69.00	23280.0
70.00	2240.0
71.10	125.0
72.00	1212.0
73.00	10244.0
74.00	39304.0
75.00	114288.0
76.00	9460.0
77.00	1416.0
77.90	648.0
78.90	7909.0
79.90	2445.0
80.90	8256.0
81.90	1833.0
83.00	242.0
86.00	231.0
87.00	8168.0
87.90	8326.0
90.10	119.0
90.90	909.0
92.00	6397.0
93.00	9075.0
94.00	25976.0
95.00	208576.0
96.00	13068.0
97.00	465.0
102.80	103.0
103.90	1118.0
104.90	323.0
105.90	990.0
106.90	258.0
109.90	192.0
110.90	327.0
111.80	271.0
112.90	281.0
114.70	270.0
115.80	771.0
116.90	1381.0
117.90	716.0
118.90	1249.0
122.00	138.0
123.90	169.0
127.80	770.0
128.90	475.0
129.90	867.0
131.00	269.0
134.90	476.0
136.90	422.0
140.10	191.0
140.90	2380.0
142.10	331.0
143.00	2729.0
144.10	216.0
144.90	302.0
145.90	290.0
147.00	216.0
147.90	483.0
149.00	185.0
149.90	321.0
152.00	120.0
152.90	183.0
154.00	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

154.80	422.0
155.90	133.0
156.90	341.0
157.90	101.0
158.80	260.0
160.90	247.0
171.00	229.0
171.90	912.0
173.00	1618.0
174.00	144768.0
175.00	10411.0
176.00	137728.0
177.00	9081.0
178.10	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

Scan 2782 (10.035 min): VV019870.D
BFB76

m/z	Abundance
35.80	123.0
40.00	362.0
41.40	106.0
42.20	102.0
43.20	136.0
43.90	708.0
69.10	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76