

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123021\
 Data File : VV024234.D
 Acq On : 30 Dec 2021 11:04
 Operator : SY/MD
 Sample : VV1230WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK286

Quant Time: Dec 31 03:49:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 31 03:39:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	81874	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	84516	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	44138	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	32707	5.311	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	106.200%	
7) Chloroethane-d5	1.568	69	26095	5.081	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.600%	
11) 1,1-Dichloroethene-d2	2.108	63	48992	3.273	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.400%	
20) 2-Butanone-d5	3.912	46	36962	54.033	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	108.060%	
24) Chloroform-d	4.346	84	62529	4.783	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.600%	
26) 1,2-Dichloroethane-d4	5.034	65	31208	5.333	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.600%	
32) Benzene-d6	5.050	84	120050	5.260	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.200%	
36) 1,2-Dichloropropane-d6	6.069	67	33713	5.393	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	107.800%	
41) Toluene-d8	7.317	98	109645	4.874	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.400%	
43) trans-1,3-Dichloroprop...	7.622	79	13106	4.951	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	99.000%	
46) 2-Hexanone-d5	8.092	63	42954	48.257	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.520%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	22427	5.254	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	43058	5.612	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.200%	
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	4277	0.356	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123021\
Data File : VV024234.D
Acq On : 30 Dec 2021 11:04
Operator : SY/MD
Sample : VV1230WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Quant Time: Dec 31 03:49:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 31 03:39:03 2021
Response via : Initial Calibration

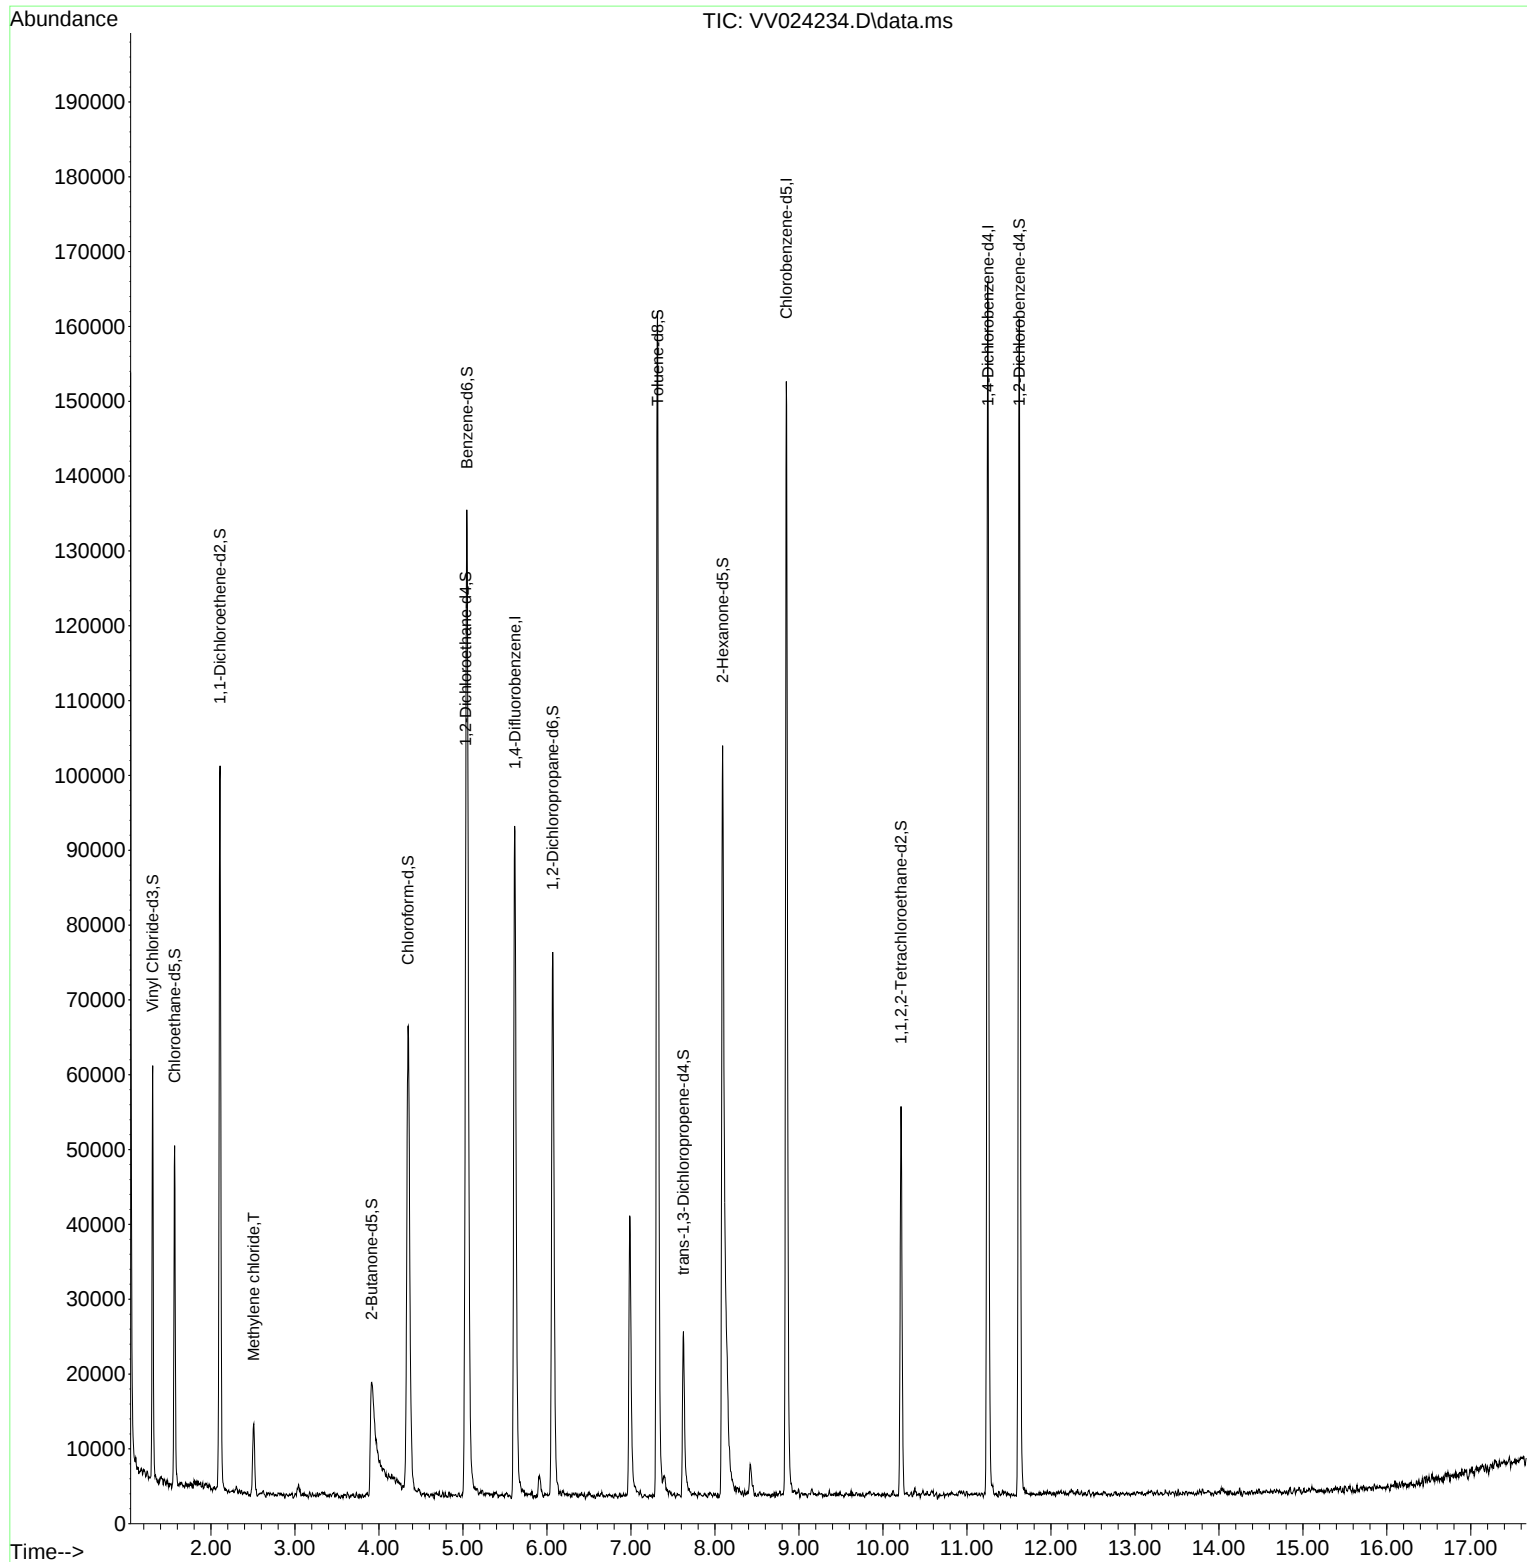

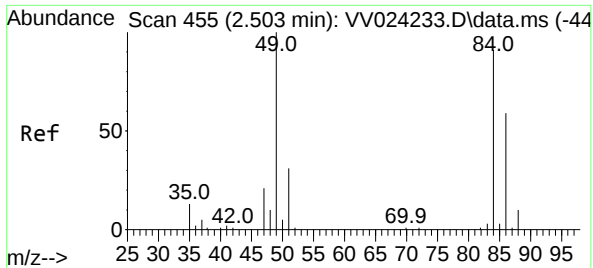

#16
Methylene chloride
Concen: 0.356 ug/L
RT: 2.510 min Scan# 41
Delta R.T. 0.007 min
Lab File: VV024234.D
Acq: 30 Dec 2021 11:04

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Tgt Ion: 84 Resp: 4277
Ion Ratio Lower Upper
84 100
86 61.6 42.6 79.0
49 100.9 79.7 147.9

