

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW123021\
 Data File : VW024239.D
 Acq On : 30 Dec 2021 13:17
 Operator : SY/MD
 Sample : M5193-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Dec 31 04:15:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 31 03:39:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	75484	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	79533	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	40175	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	31653	5.575	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	111.600%	
7) Chloroethane-d5	1.565	69	24959	5.271	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	105.400%	
11) 1,1-Dichloroethene-d2	2.105	63	46220	3.349	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.000%	
20) 2-Butanone-d5	3.902	46	30791	48.822	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	97.640%	
24) Chloroform-d	4.346	84	62435	5.180	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.600%	
26) 1,2-Dichloroethane-d4	5.031	65	30358	5.627	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	112.600%	
32) Benzene-d6	5.047	84	113698	5.294	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.800%	
36) 1,2-Dichloropropane-d6	6.066	67	31787	5.403	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	108.000%	
41) Toluene-d8	7.314	98	104060	4.916	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.400%	
43) trans-1,3-Dichloroprop...	7.622	79	13009	5.222	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	104.400%	
46) 2-Hexanone-d5	8.088	63	46834	55.913	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	111.820%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	23445	5.837	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	116.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	40301	5.771	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	115.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	4479	0.404	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123021\
Data File : VV024239.D
Acq On : 30 Dec 2021 13:17
Operator : SY/MD
Sample : M5193-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Dec 31 04:15:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 31 03:39:03 2021
Response via : Initial Calibration

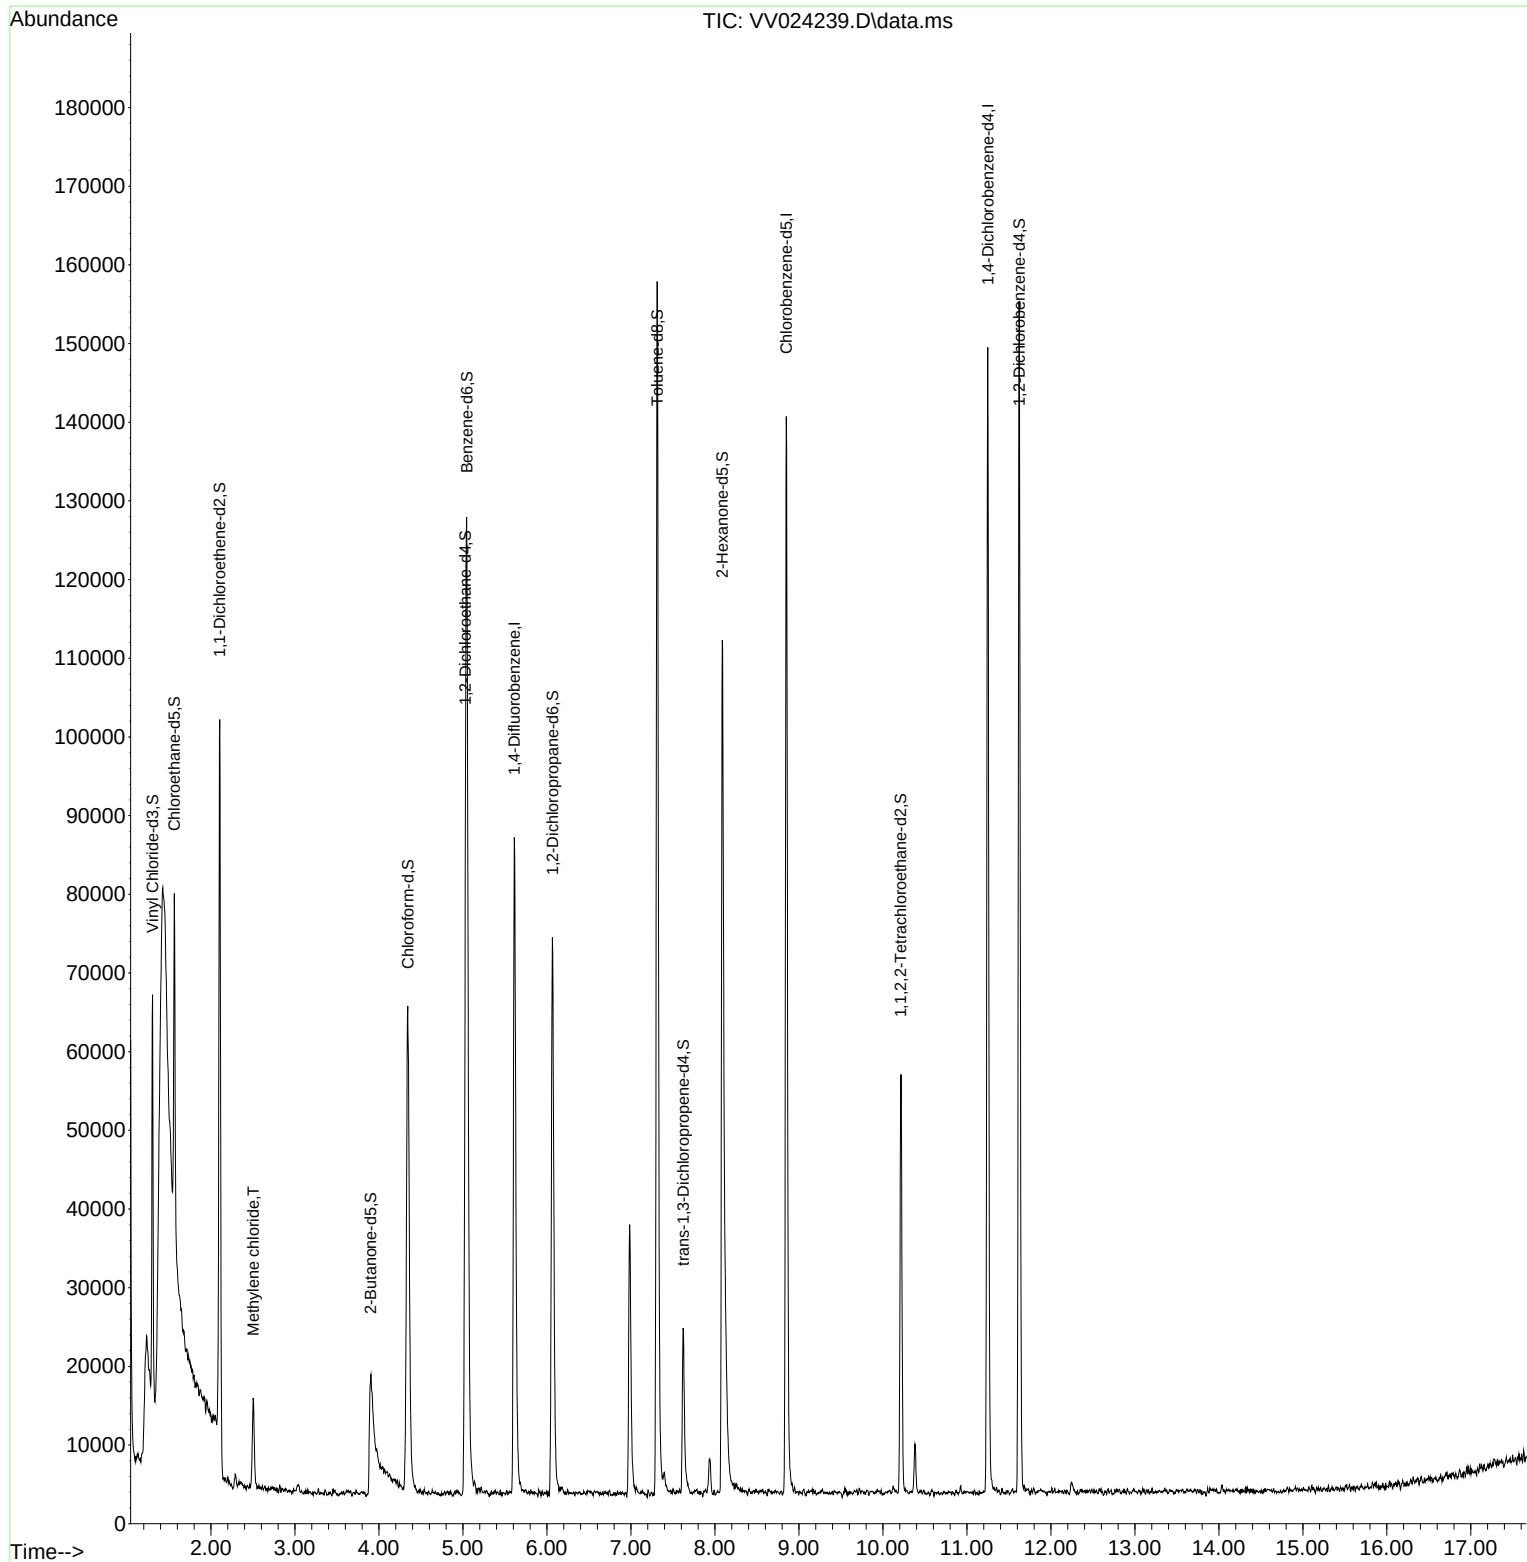

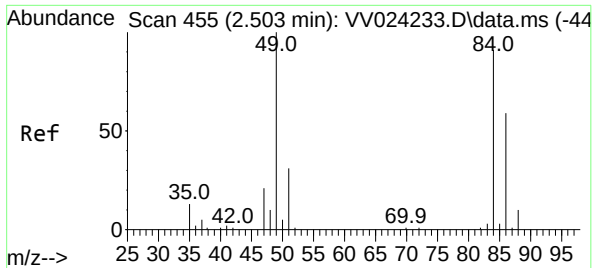

#16
Methylene chloride
Concen: 0.404 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV024239.D
Acq: 30 Dec 2021 13:17

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	4479
Ion	Ratio	Lower	Upper
84	100		
86	64.5	42.6	79.0
49	105.1	79.7	147.9

