

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123021\
 Data File : VV024234.D
 Acq On : 30 Dec 2021 11:04
 Operator : SY/MD
 Sample : VV1230WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK286

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	91	rVB	54904	54770	16.80%	2.089%
2	1.568	153	164	177	rBV	45825	53649	16.46%	2.046%
3	2.108	322	332	350	rVB	96843	138431	42.47%	5.279%
4	2.510	444	457	470	rBV3	9703	17213	5.28%	0.656%
5	3.915	882	894	909	rBV	15226	51257	15.73%	1.955%
6	4.349	1013	1029	1051	rVB	61845	153049	46.96%	5.837%
7	5.047	1230	1246	1272	rBV3	131701	325918	100.00%	12.430%
8	5.616	1410	1423	1448	rBV2	89896	187758	57.61%	7.161%
9	5.912	1506	1515	1522	rBV5	2880	5467	1.68%	0.208%
10	6.069	1552	1564	1587	rBV2	72506	150018	46.03%	5.721%
11	6.985	1837	1849	1866	rBV	37450	69345	21.28%	2.645%
12	7.317	1940	1952	1970	rBV	158430	282878	86.79%	10.788%
13	7.625	2039	2048	2066	rBV	22127	40744	12.50%	1.554%
14	8.092	2179	2193	2237	rBV	100534	256584	78.73%	9.786%
15	8.420	2287	2295	2304	rBV3	3939	6705	2.06%	0.256%
16	8.850	2417	2429	2446	rBV	148813	244575	75.04%	9.328%
17	10.217	2844	2854	2867	rBV	51958	80831	24.80%	3.083%
18	11.249	3165	3175	3189	rBV	162014	251046	77.03%	9.574%
19	11.622	3280	3291	3308	rBV	157400	251841	77.27%	9.605%




Sum of corrected areas: 2622079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123021\
Data File : VV024234.D
Acq On : 30 Dec 2021 11:04
Operator : SY/MD
Sample : VV1230WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

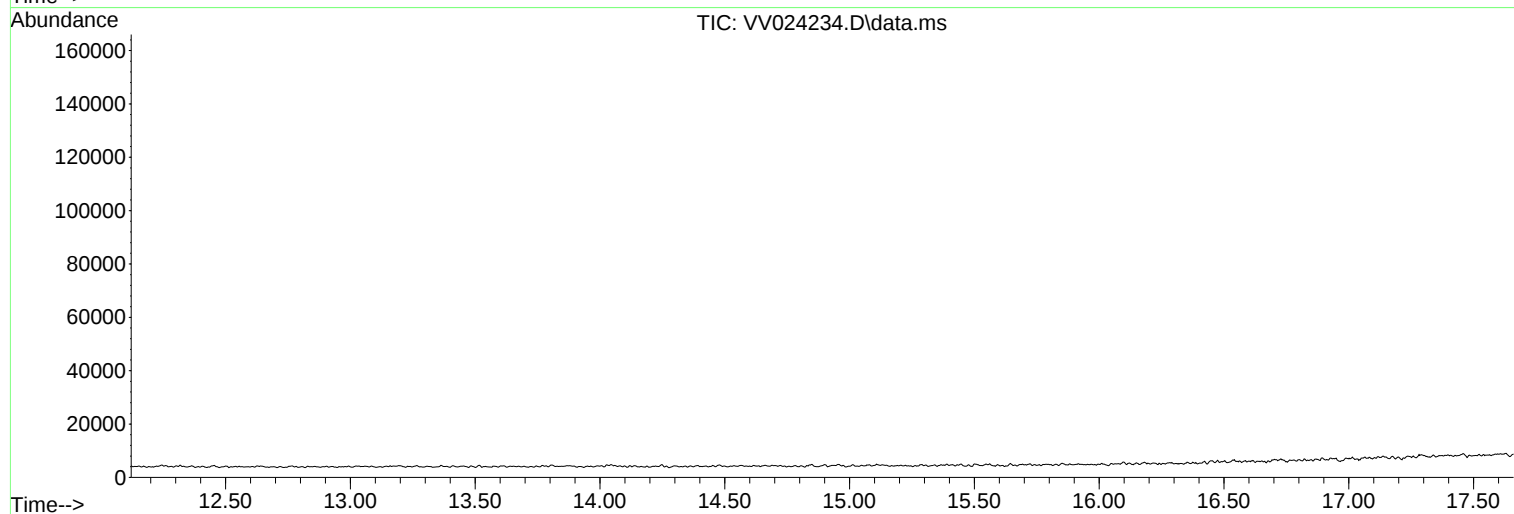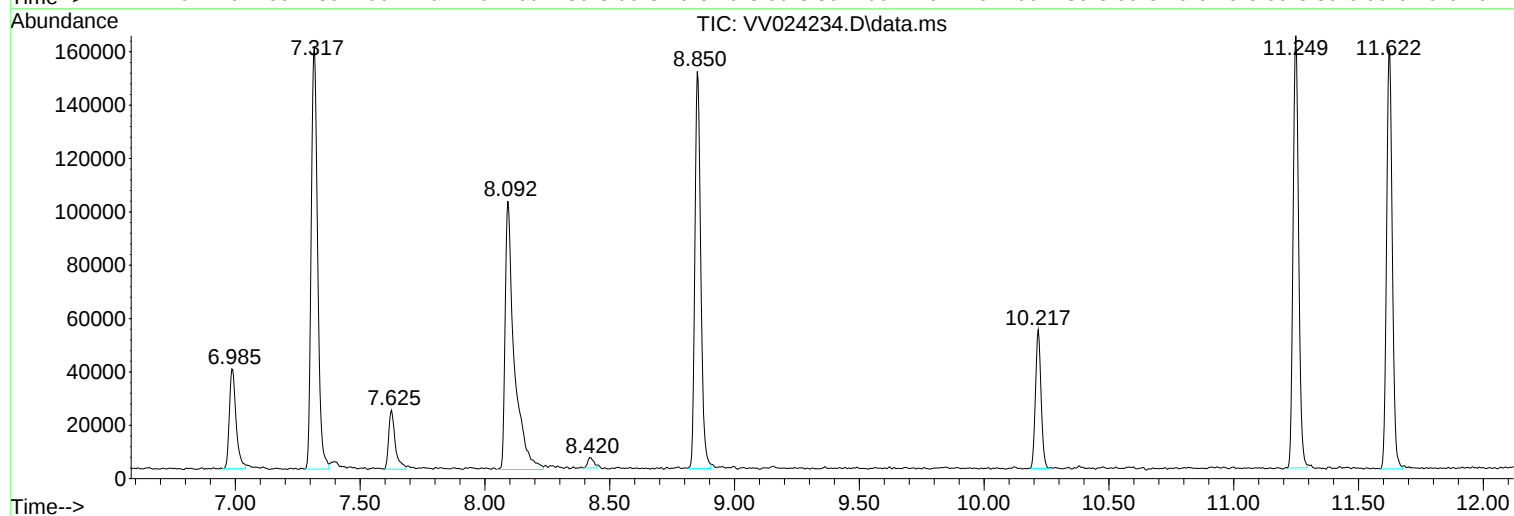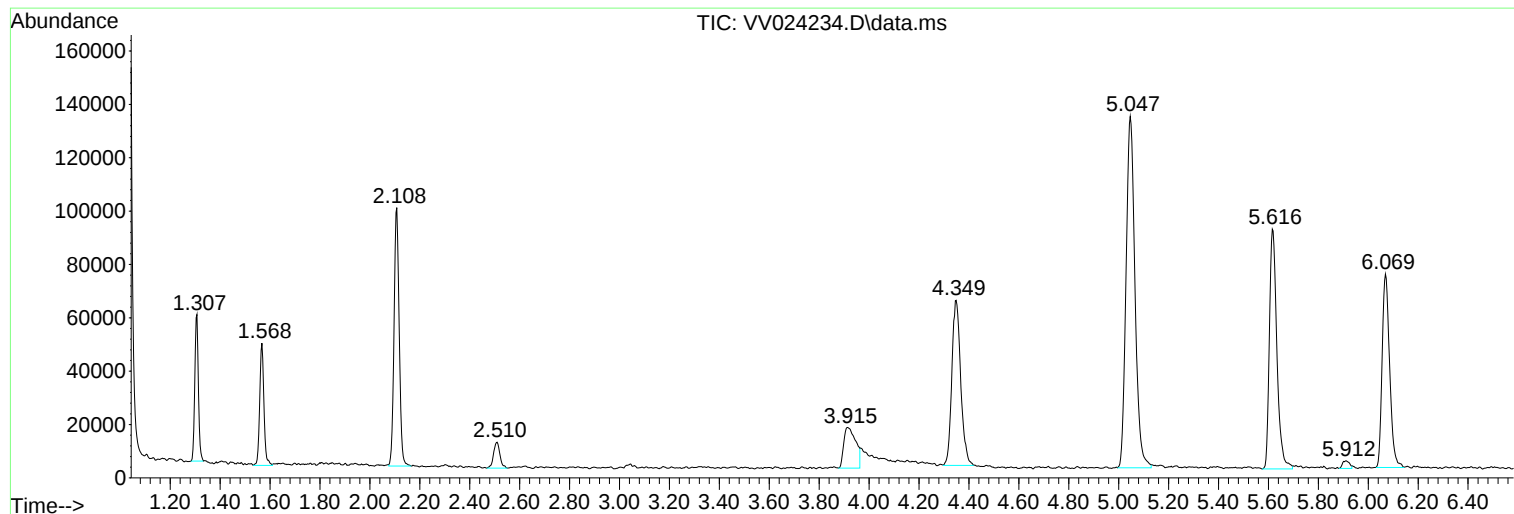

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123021\
Data File : VV024234.D
Acq On : 30 Dec 2021 11:04
Operator : SY/MD
Sample : VV1230WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123021\
Data File : VV024234.D
Acq On : 30 Dec 2021 11:04
Operator : SY/MD
Sample : VV1230WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc