
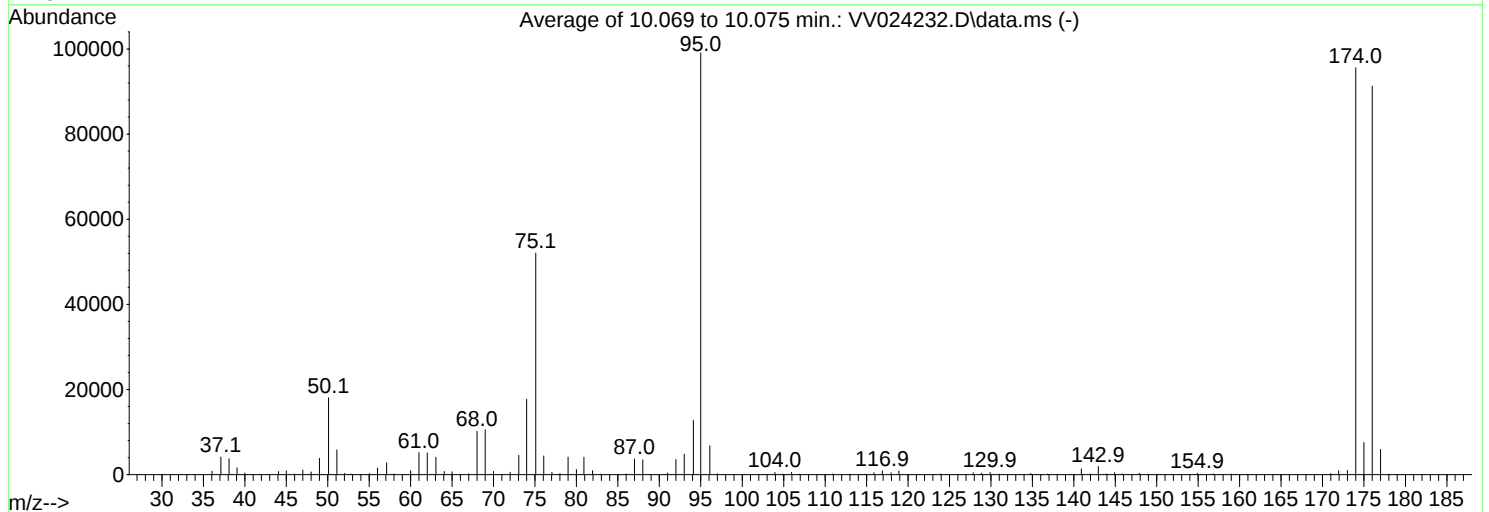


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123021\
 Data File : VV024232.D
 Acq On : 30 Dec 2021 08:30
 Operator : SY/MD
 Sample : BFB258
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB258

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Dec 31 03:39:03 2021

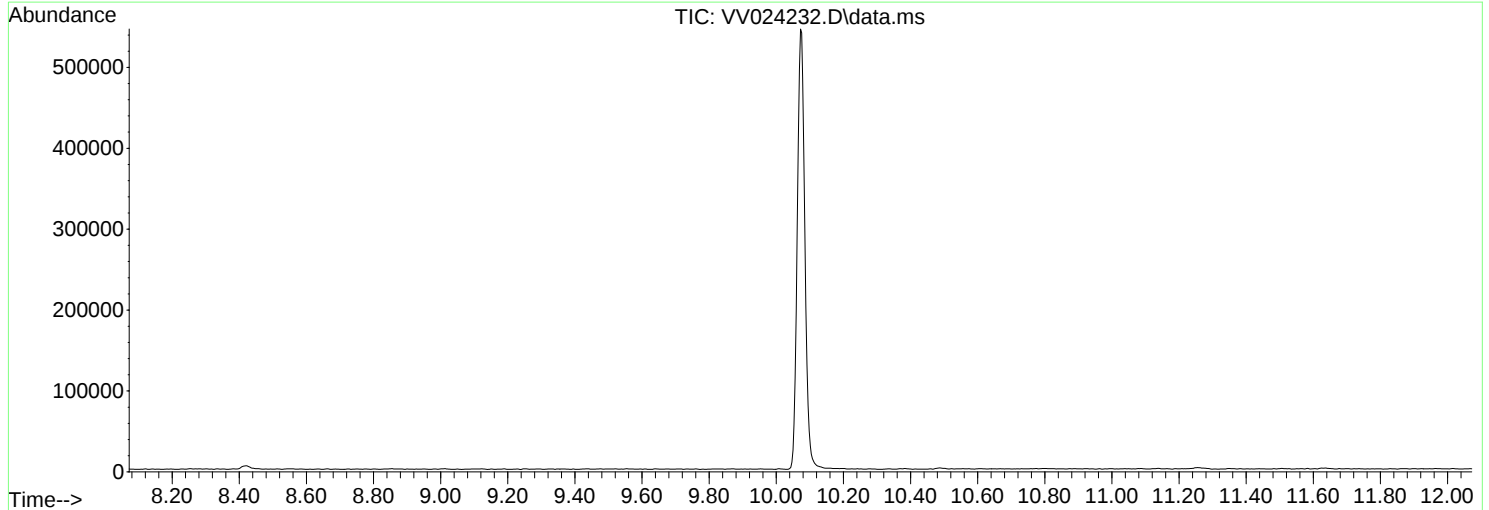

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	18096	PASS
75	95	30	80	52.6	52072	PASS
95	95	100	100	100.0	99088	PASS
96	95	5	9	6.8	6773	PASS
173	174	0.00	2	1.0	983	PASS
174	95	50	120	96.5	95600	PASS
175	174	5	9	7.9	7571	PASS
176	174	95	105	95.5	91283	PASS
177	176	5	10	6.5	5943	PASS

m/z	Abundance
40.00	3130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
36.00	826.0
37.10	3936.0
38.10	3570.0
39.10	1579.0
40.00	3501.0
44.00	651.0
45.00	847.0
46.00	170.0
47.00	1111.0
48.00	643.0
49.00	3744.0
50.10	17520.0
51.10	5472.0
52.00	319.0
52.90	124.0
53.90	132.0
55.10	309.0
56.00	1602.0
57.10	2678.0
58.00	169.0
60.00	826.0
61.00	4877.0
62.00	4700.0
63.00	4018.0
64.00	767.0
65.00	613.0
67.00	202.0
68.00	9212.0
69.00	9952.0
70.00	731.0
72.10	529.0
73.00	4193.0
74.00	17096.0
75.10	49256.0
76.00	4321.0
77.00	579.0
78.00	231.0
79.00	4010.0
80.00	1200.0
80.90	4029.0
82.00	895.0
82.90	119.0
86.00	189.0
87.00	3596.0
88.00	3185.0
91.00	418.0
92.00	3265.0
93.00	4521.0
94.10	11888.0
95.00	94288.0
96.10	6530.0
97.00	262.0
102.80	102.0
104.00	508.0
104.90	151.0
105.90	468.0
106.90	103.0
109.90	105.0
110.90	168.0
112.90	119.0
115.00	114.0
115.90	406.0
116.90	777.0
117.90	442.0
118.90	801.0
123.90	153.0
127.90	440.0
128.90	308.0
129.90	487.0
131.00	141.0
134.80	285.0
136.90	144.0
140.90	1304.0
141.90	183.0
142.90	1867.0
143.90	211.0
144.90	374.0
145.80	170.0
147.90	286.0
148.90	128.0
150.00	119.0
154.90	281.0
156.90	210.0
159.00	118.0
160.80	109.0
171.00	253.0
171.90	787.0
174.00	88888.0
175.00	7019.0
176.00	84264.0
177.00	5520.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
36.10	857.0
37.10	4237.0
38.10	3860.0
39.10	1671.0
40.00	3491.0
44.10	723.0
45.00	962.0
46.00	154.0
47.00	1153.0
48.00	669.0
49.00	3892.0
50.10	18800.0
51.10	6089.0
52.00	342.0
52.90	127.0
53.90	119.0
55.00	279.0
56.00	1576.0
57.10	2843.0
58.00	153.0
60.00	953.0
61.00	5308.0
62.00	5297.0
63.10	4253.0
64.00	765.0
65.00	702.0
67.00	233.0
68.00	10559.0
69.00	11001.0
70.00	809.0
72.00	578.0
73.10	4637.0
74.00	18352.0
75.10	53984.0
76.10	4568.0
77.10	593.0
78.00	268.0
79.00	4250.0
80.00	1261.0
80.90	4230.0
82.00	1004.0
82.90	122.0
86.00	226.0
87.00	3843.0
88.00	3565.0
91.00	423.0
92.00	3712.0
93.00	4937.0
94.10	13211.0
95.00	102416.0
96.10	7025.0
97.00	222.0
104.00	571.0
104.90	170.0
105.90	531.0
106.90	109.0
110.90	165.0
113.00	131.0
114.90	120.0
115.90	483.0
116.90	923.0
118.00	434.0
118.90	913.0
123.90	155.0
127.80	479.0
128.90	298.0
129.90	559.0
131.00	161.0
134.80	308.0
136.90	168.0
140.90	1389.0
141.90	212.0
142.90	1969.0
143.90	210.0
144.90	499.0
145.80	191.0
147.90	327.0
148.90	104.0
150.00	124.0
154.90	381.0
156.80	184.0
159.00	144.0
160.80	106.0
171.00	284.0
172.00	916.0
173.00	1454.0
174.00	98640.0
175.00	7798.0
176.00	94304.0
177.00	6124.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
36.10	811.0
37.10	4224.0
38.10	3808.0
39.00	1624.0
40.00	3534.0
44.10	748.0
45.00	926.0
45.90	110.0
47.00	1044.0
48.00	630.0
49.00	3823.0
50.10	17968.0
51.10	5921.0
52.10	298.0
52.90	102.0
55.00	236.0
56.00	1479.0
57.10	2797.0
58.00	152.0
60.00	1028.0
61.00	5348.0
62.00	5362.0
63.10	4044.0
64.10	709.0
65.00	675.0
65.90	121.0
67.00	237.0
68.00	10768.0
69.00	10740.0
70.00	767.0
71.90	615.0
73.10	4809.0
74.00	17720.0
75.10	52976.0
76.10	4298.0
77.00	526.0
78.00	309.0
79.00	4106.0
80.00	1125.0
80.90	4097.0
81.90	972.0
83.00	118.0
86.00	192.0
87.00	3659.0
88.00	3774.0
91.00	426.0
92.00	3728.0
93.00	4923.0
94.10	13287.0
95.00	100560.0
96.10	6763.0
97.00	177.0
103.90	552.0
104.80	139.0
106.00	552.0
106.90	110.0
110.90	152.0
113.00	147.0
114.80	132.0
115.90	511.0
116.90	943.0
118.00	453.0
118.90	835.0
123.90	128.0
127.80	470.0
128.80	251.0
129.90	545.0
131.00	158.0
134.80	266.0
136.80	190.0
140.90	1364.0
142.00	216.0
143.00	1868.0
143.90	193.0
144.90	506.0
145.80	202.0
147.90	329.0
150.00	136.0
154.90	399.0
156.90	149.0
159.00	149.0
171.00	289.0
172.00	1000.0
173.00	1494.0
174.00	99272.0
175.00	7895.0
176.00	95280.0
177.00	6185.0
178.00	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258