

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV123119\
 Data File : VV014243.D
 Acq On : 31 Dec 2019 17:04
 Operator : SY/MD
 Sample : VIBLK45
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK45

Quant Time: Jan 01 10:38:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jan 01 03:03:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	817605	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	741622	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	336704	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	309882	8.09	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	161.80%#
7) Chloroethane-d5	1.58	69	234121	7.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	146.80%#
11) 1,1-Dichloroethene-d2	2.13	63	368656	5.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	107.20%
20) 2-Butanone-d5	3.94	46	714691	75.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	150.28%#
24) Chloroform-d	4.40	84	512278	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
26) 1,2-Dichloroethane-d4	5.08	65	285675	6.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.40%
32) Benzene-d6	5.10	84	1196161	5.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	118.00%
36) 1,2-Dichloropropane-d6	6.11	67	370653	6.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	121.00%
41) Toluene-d8	7.36	98	1090012	5.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.20%
43) trans-1,3-Dichloropropene-	7.66	79	157079	5.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	114.60%
46) 2-Hexanone-d5	8.13	63	622590	59.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.66%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	244298	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	342692	5.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.60%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	11624	0.191 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV123119\
Data File : VV014243.D
Acq On : 31 Dec 2019 17:04
Operator : SY/MD
Sample : VIBLK45
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK45

Quant Time: Jan 01 10:38:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jan 01 03:03:23 2020
Response via : Initial Calibration

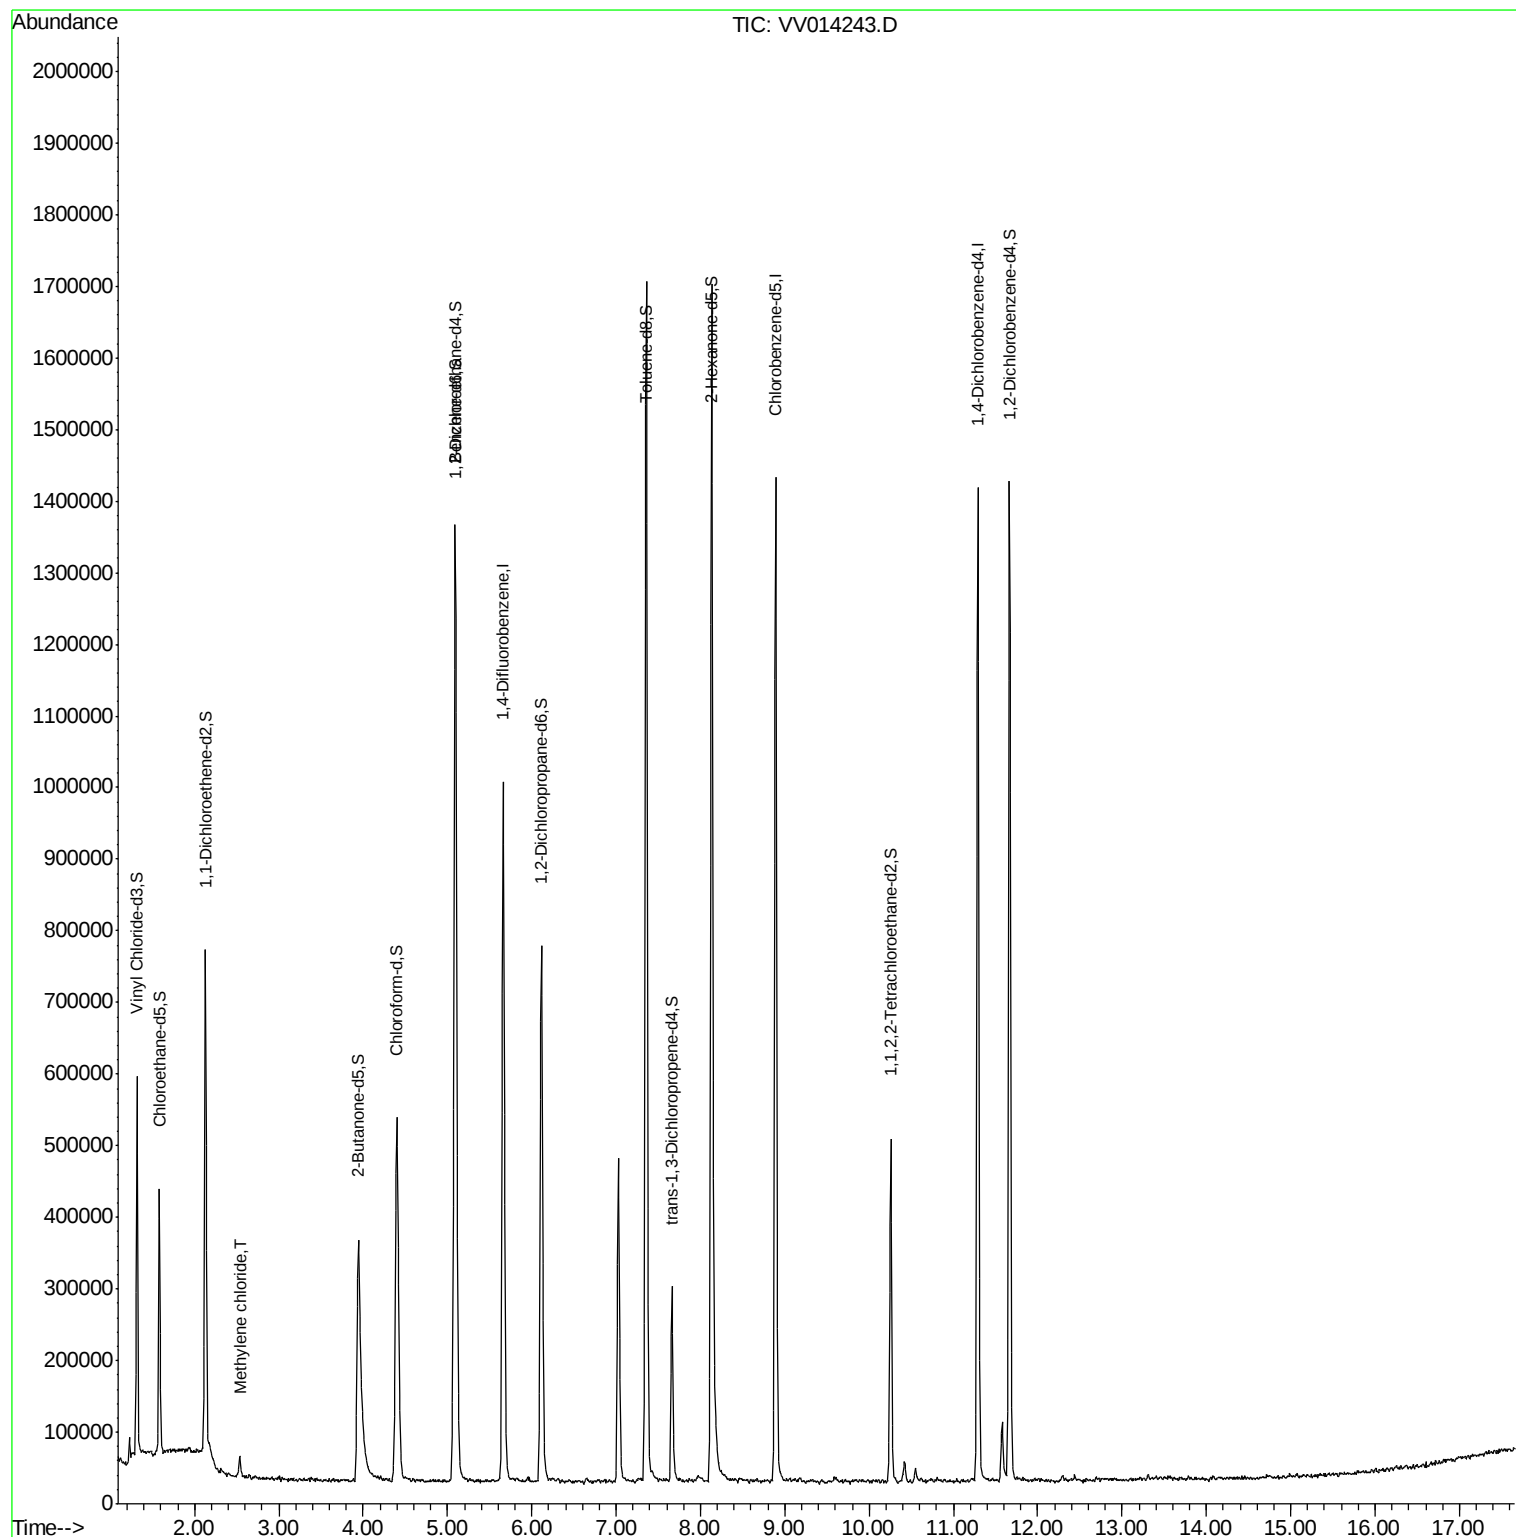

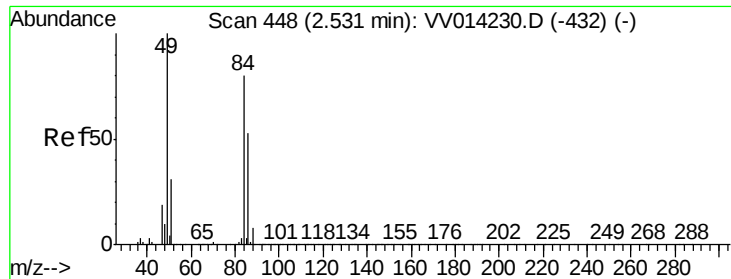

#16
 Methvlene chloride
 Concen: 0.191 ug/L
 RT: 2.54 min Scan# 450
 Delta R.T. 0.01 min
 Lab File: VV014243.D
 Acq: 31 Dec 2019 17:04

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK45

Tot Ion: 84 Resp: 11624
 Ion Ratio Lower Upper
 84 100
 86 56.8 43.1 80.1
 49 107.2 82.1 152.5

