
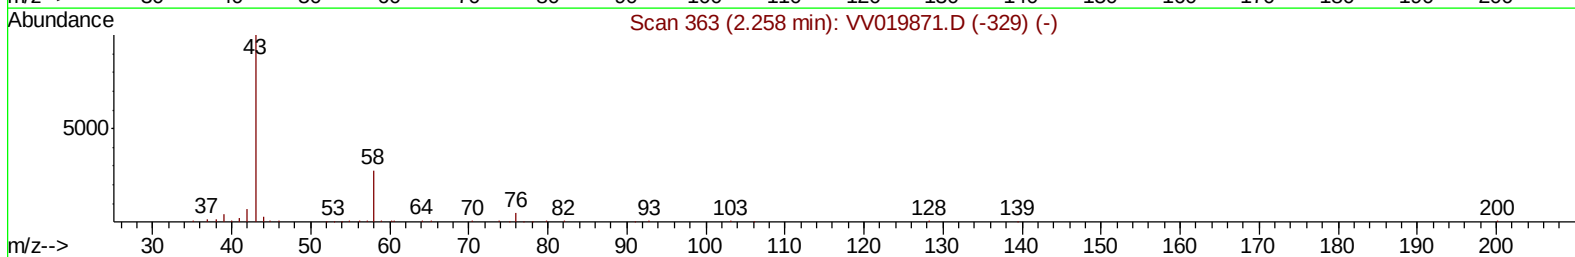
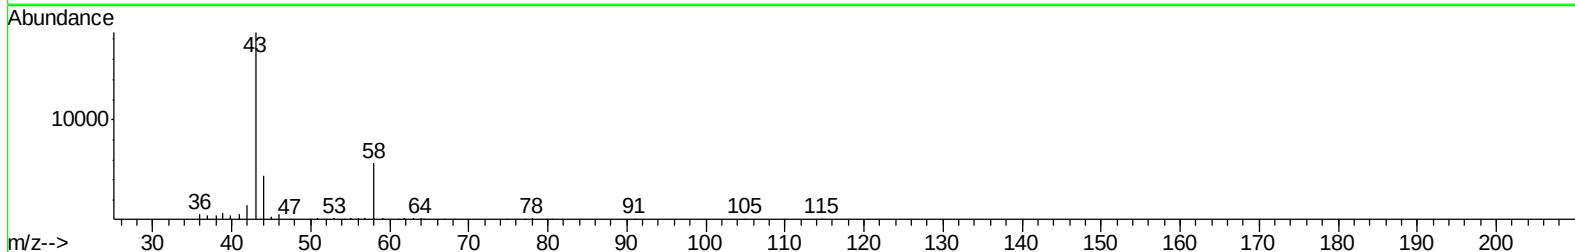


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV123120\
Data File : VV019878.D
Acq On : 31 Dec 2020 13:37
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jan 01 00:33:19 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR122920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 31 02:03:35 2020
Response via : Initial Calibration

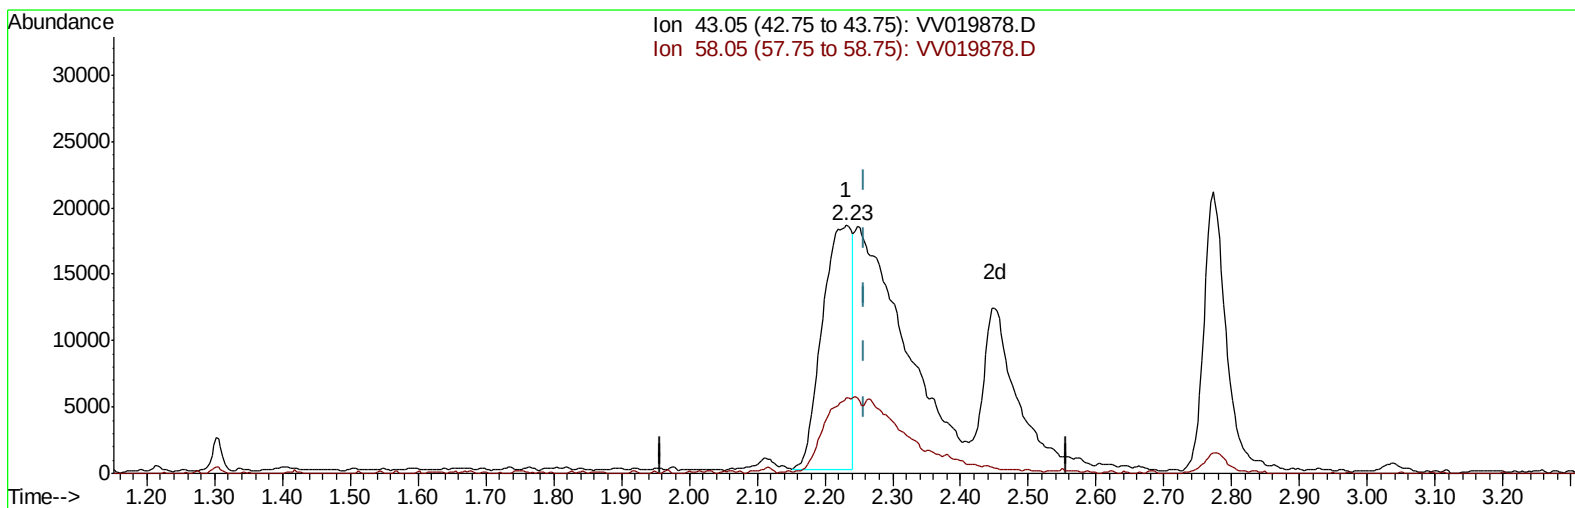

TIC: VV019878.D

(13) Acetone (T)

2.232min (-0.026) 17.64ug/L

response 56230

Ion	Exp%	Act%
43.05	100	100
58.05	15.70	36.23#
0.00	0.00	0.00
0.00	0.00	0.00