


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV123120\
 Data File : VV019877.D
 Acq On : 31 Dec 2020 13:07
 Operator : SY/MD
 Sample : BFB77
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB77

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR122920WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Jan 01 00:38:14 2021

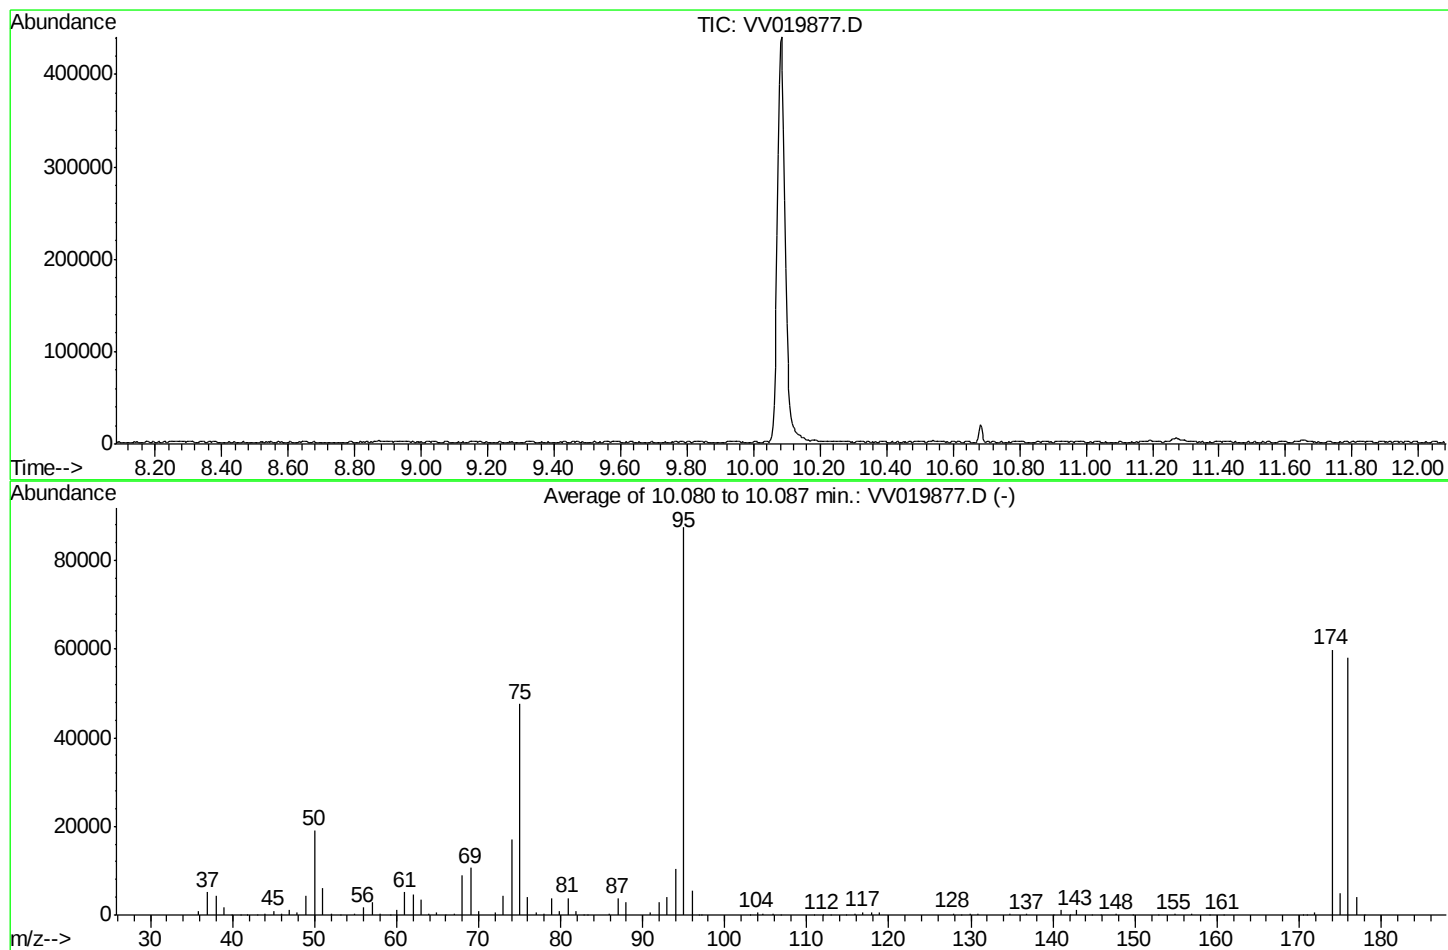

AutoFind: Scans 2796, 2797, 2798; Background Corrected with Scan 2783

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	18936	PASS
75	95	30	80	54.3	47538	PASS
95	95	100	100	100.0	87480	PASS
96	95	5	9	6.4	5604	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.5	59901	PASS
175	174	5	9	8.0	4818	PASS
176	174	95	105	97.1	58157	PASS
177	176	5	10	7.1	4146	PASS

m/z	Abundance
35.90	1008.0
37.00	5336.0
38.00	4553.0
39.00	1905.0
40.00	404.0
41.80	164.0
43.00	148.0
44.00	1347.0
45.00	970.0
46.00	190.0
47.00	1321.0
47.90	646.0
49.00	4482.0
50.00	19464.0
51.00	6570.0
52.10	378.0
54.90	322.0
56.00	1762.0
57.00	2837.0
58.00	258.0
59.20	114.0
60.00	1145.0
61.00	5225.0
62.00	4651.0
63.00	3610.0
63.90	384.0
64.90	495.0
67.10	388.0
68.00	9426.0
69.00	11065.0
70.00	873.0
71.90	693.0
73.00	4368.0
74.00	17384.0
75.00	48864.0
76.00	4065.0
76.90	612.0
77.90	506.0
78.90	3906.0
79.80	916.0
80.90	3923.0
81.80	716.0
83.20	110.0
85.90	174.0
87.00	3671.0
87.90	3045.0
91.00	484.0
92.00	3094.0
93.00	4478.0
94.00	10862.0
95.00	90112.0
96.00	5926.0
96.90	121.0
103.90	458.0
104.70	195.0
105.80	439.0
111.90	138.0
112.90	139.0
114.80	103.0
115.80	413.0
116.90	610.0
117.80	423.0
118.90	635.0
127.90	349.0
128.70	146.0
129.90	258.0
130.80	178.0
134.80	197.0
136.90	205.0
140.00	110.0
141.00	1156.0
142.80	1012.0
145.90	143.0
147.80	195.0
149.70	150.0
154.90	274.0
157.00	203.0
160.80	135.0
171.00	151.0
171.90	414.0
174.00	60200.0
175.00	4914.0
176.00	57760.0
176.90	4153.0
178.00	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	866.0
37.00	5240.0
38.00	4528.0
39.00	1799.0
39.90	403.0
41.00	105.0
41.80	140.0
43.00	134.0
44.00	1311.0
45.00	990.0
45.90	181.0
47.00	1263.0
47.90	702.0
49.00	4647.0
50.00	19544.0
51.00	6414.0
52.00	327.0
54.90	324.0
56.00	1645.0
57.00	2883.0
58.00	240.0
60.00	1269.0
61.00	5280.0
62.00	4622.0
63.00	3668.0
63.90	412.0
64.90	518.0
67.10	402.0
68.00	9336.0
69.00	10942.0
69.90	790.0
71.90	611.0
73.00	4398.0
74.00	17536.0
75.00	48984.0
76.00	4162.0
77.00	656.0
77.90	453.0
78.90	3974.0
79.80	932.0
80.90	3907.0
81.80	813.0
82.80	131.0
83.20	140.0
85.90	202.0
87.00	3731.0
87.90	3038.0
90.90	552.0
92.00	3140.0
93.00	4325.0
94.00	10695.0
95.00	90336.0
96.00	5767.0
96.90	110.0
103.00	124.0
104.00	492.0
104.70	214.0
105.90	443.0
110.80	107.0
111.90	121.0
112.90	129.0
115.80	415.0
116.90	701.0
117.80	476.0
118.90	611.0
127.90	335.0
128.80	134.0
129.90	291.0
130.80	192.0
134.80	209.0
136.80	226.0
140.00	125.0
141.00	1144.0
142.00	109.0
142.90	1195.0
144.70	104.0
145.80	156.0
147.80	174.0
149.80	102.0
152.90	104.0
154.80	275.0
157.00	202.0
160.80	145.0
171.80	482.0
174.00	61992.0
175.00	4997.0
176.00	60184.0
177.00	4273.0
177.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	705.0
37.00	4765.0
38.00	4109.0
39.00	1594.0
39.90	427.0
41.00	102.0
41.80	113.0
43.20	118.0
43.90	1307.0
45.00	928.0
46.00	168.0
46.90	1090.0
47.90	629.0
49.00	4301.0
50.00	17800.0
51.00	5668.0
51.90	281.0
53.20	139.0
54.90	326.0
55.90	1462.0
57.00	2593.0
58.00	186.0
60.00	1217.0
61.00	4906.0
62.00	4330.0
63.00	3505.0
63.90	412.0
64.90	449.0
66.00	115.0
67.10	395.0
68.00	8506.0
69.00	9788.0
70.00	762.0
72.00	555.0
73.00	3959.0
74.00	15902.0
75.00	44768.0
76.00	3857.0
76.90	616.0
77.90	346.0
78.90	3523.0
79.90	951.0
80.90	3553.0
81.80	875.0
82.80	145.0
83.20	169.0
85.80	169.0
87.00	3485.0
87.90	2916.0
90.90	583.0
92.00	2787.0
93.00	3708.0
94.00	9821.0
95.00	81992.0
96.00	5120.0
97.20	145.0
103.00	118.0
103.90	512.0
104.70	196.0
105.90	438.0
106.80	111.0
110.80	119.0
113.00	114.0
115.80	381.0
116.80	721.0
117.90	463.0
118.90	542.0
127.80	305.0
128.90	140.0
129.90	322.0
130.80	201.0
134.80	208.0
136.90	238.0
140.10	126.0
141.00	1005.0
142.00	107.0
142.90	1162.0
144.70	147.0
145.80	166.0
147.70	161.0
152.80	100.0
154.80	223.0
156.90	159.0
159.10	111.0
160.80	182.0
170.50	102.0
171.80	500.0
174.00	57512.0
175.00	4544.0
176.00	56528.0
177.00	4013.0
177.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.50	190.0
39.00	159.0
39.90	375.0
40.60	103.0
41.90	102.0
43.20	215.0
44.00	927.0
46.40	144.0
48.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77