

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
 Data File : VV024251.D
 Acq On : 30 Dec 2021 23:33
 Operator : SY/MD
 Sample : M5194-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

Signal : TIC: VV024251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	146250	145301	16.76%	2.122%
2	1.568	157	164	176	rBV	111853	122273	14.10%	1.786%
3	2.108	322	332	358	rVB	249917	365375	42.14%	5.336%
4	2.558	470	472	474	rBV	528	251	0.03%	0.004%
5	2.892	572	576	580	rBV	929	726	0.08%	0.011%
6	3.056	623	627	629	rBV	587	471	0.05%	0.007%
7	3.545	776	779	782	rBV2	559	462	0.05%	0.007%
8	3.625	802	804	807	rBV	378	264	0.03%	0.004%
9	3.696	823	826	827	rBV	483	302	0.03%	0.004%
10	3.847	867	873	874	rBV2	788	709	0.08%	0.010%
11	3.886	875	885	914	rVV	50559	158915	18.33%	2.321%
12	4.342	1013	1027	1054	rBV	147584	363911	41.97%	5.315%
13	4.481	1065	1070	1076	rBV3	769	994	0.11%	0.015%
14	4.539	1084	1088	1089	rBV	284	180	0.02%	0.003%
15	4.548	1089	1091	1095	rVB3	621	387	0.04%	0.006%
16	4.580	1097	1101	1105	rBV	817	782	0.09%	0.011%
17	4.719	1139	1144	1150	rBV2	655	777	0.09%	0.011%
18	4.748	1150	1153	1156	rBV	388	323	0.04%	0.005%
19	4.786	1161	1165	1169	rBV	874	830	0.10%	0.012%
20	4.815	1172	1174	1176	rBV	404	169	0.02%	0.002%
21	4.870	1187	1191	1193	rBV2	458	400	0.05%	0.006%
22	4.902	1198	1201	1204	rBV	533	325	0.04%	0.005%
23	4.957	1214	1218	1222	rBV	809	728	0.08%	0.011%
24	5.043	1228	1245	1274	rBV2	334234	867073	100.00%	12.663%
25	5.246	1306	1308	1310	rBV	498	290	0.03%	0.004%
26	5.320	1329	1331	1334	rBV2	403	194	0.02%	0.003%
27	5.494	1380	1385	1391	rBV2	910	1049	0.12%	0.015%
28	5.612	1411	1422	1440	rBV	281643	559164	64.49%	8.167%
29	5.905	1503	1513	1528	rBV3	9644	18899	2.18%	0.276%
30	6.066	1550	1563	1583	rBV2	183092	371560	42.85%	5.427%
31	6.227	1610	1613	1619	rBV2	754	675	0.08%	0.010%
32	6.272	1624	1627	1634	rVB	403	480	0.06%	0.007%
33	6.307	1634	1638	1644	rVB	920	1007	0.12%	0.015%
34	6.349	1647	1651	1653	rBV2	599	487	0.06%	0.007%
35	6.362	1653	1655	1659	rBV	344	260	0.03%	0.004%
36	6.458	1683	1685	1688	rVB	314	145	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW123121\
 Data File : VW024251.D
 Acq On : 30 Dec 2021 23:33
 Operator : SY/MD
 Sample : M5194-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	6.638	1738	1741	1744	rBV2	437	317	0.04%	0.005%
38	6.715	1759	1765	1770	rBV2	521	647	0.07%	0.009%
39	6.757	1775	1778	1782	rVV	572	416	0.05%	0.006%
40	6.899	1819	1822	1824	rBV	456	278	0.03%	0.004%
41	6.982	1835	1848	1867	rBV	109084	199785	23.04%	2.918%
42	7.243	1927	1929	1931	rBV	335	150	0.02%	0.002%
43	7.265	1931	1936	1939	rBV	692	777	0.09%	0.011%
44	7.313	1939	1951	1969	rBV	420323	719647	83.00%	10.510%
45	7.474	1999	2001	2005	rBV4	755	436	0.05%	0.006%
46	7.619	2036	2046	2067	rBV	79150	139868	16.13%	2.043%
47	7.879	2125	2127	2129	rBV	259	148	0.02%	0.002%
48	7.973	2150	2156	2159	rBV	647	631	0.07%	0.009%
49	7.985	2159	2160	2165	rVB	463	300	0.03%	0.004%
50	8.011	2165	2168	2171	rBV2	582	488	0.06%	0.007%
51	8.085	2181	2191	2228	rBV	195231	366499	42.27%	5.353%
52	8.300	2255	2258	2260	rBV2	678	406	0.05%	0.006%
53	8.574	2340	2343	2348	rBV	910	792	0.09%	0.012%
54	8.850	2418	2429	2455	rBV	429515	678893	78.30%	9.915%
55	9.288	2562	2565	2566	rBV	519	309	0.04%	0.005%
56	9.513	2632	2635	2636	rBV	609	378	0.04%	0.006%
57	9.551	2644	2647	2649	rBV3	496	297	0.03%	0.004%
58	9.641	2670	2675	2678	rBV	661	649	0.07%	0.009%
59	9.683	2686	2688	2689	rBV	274	127	0.01%	0.002%
60	9.767	2711	2714	2715	rBV	342	154	0.02%	0.002%
61	9.934	2764	2766	2768	rBV	322	179	0.02%	0.003%
62	10.017	2789	2792	2794	rBV	666	476	0.05%	0.007%
63	10.165	2835	2838	2840	rBV2	386	251	0.03%	0.004%
64	10.214	2842	2853	2874	rVB	252726	391953	45.20%	5.724%
65	10.362	2897	2899	2900	rBV2	285	128	0.01%	0.002%
66	10.458	2926	2929	2932	rBV	679	395	0.05%	0.006%
67	10.477	2932	2935	2939	rBV2	390	375	0.04%	0.005%
68	10.635	2981	2984	2988	rBV2	566	386	0.04%	0.006%
69	10.664	2990	2993	2994	rBV	648	365	0.04%	0.005%
70	10.754	3016	3021	3024	rBV	579	610	0.07%	0.009%
71	10.844	3044	3049	3054	rVB	458	585	0.07%	0.009%
72	10.870	3054	3057	3059	rBV2	281	158	0.02%	0.002%
73	11.143	3138	3142	3148	rVB3	1174	1246	0.14%	0.018%
74	11.165	3148	3149	3150	rBV3	250	88	0.01%	0.001%
75	11.188	3151	3156	3158	rBV3	501	526	0.06%	0.008%
76	11.249	3164	3175	3196	rVB	427403	661070	76.24%	9.655%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
 Data File : VV024251.D
 Acq On : 30 Dec 2021 23:33
 Operator : SY/MD
 Sample : M5194-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

77	11.413	3223	3226	3227	rBV2	678	401	0.05%	0.006%
78	11.622	3280	3291	3308	rBV	428556	683022	78.77%	9.975%
79	11.731	3321	3325	3329	rBV4	564	523	0.06%	0.008%
80	11.992	3403	3406	3408	rBV	445	304	0.04%	0.004%
81	12.236	3476	3482	3486	rBV	850	884	0.10%	0.013%
82	12.873	3677	3680	3682	rBV	430	343	0.04%	0.005%
83	12.969	3700	3710	3712	rBV2	544	970	0.11%	0.014%
84	13.133	3759	3761	3764	rVB2	463	248	0.03%	0.004%
85	13.149	3764	3766	3769	rBV	292	197	0.02%	0.003%
86	13.863	3984	3988	3990	rBV	786	626	0.07%	0.009%
87	13.930	4005	4009	4013	rBV2	644	548	0.06%	0.008%
88	13.992	4025	4028	4031	rBV	703	527	0.06%	0.008%
89	14.066	4049	4051	4053	rBV	458	269	0.03%	0.004%
90	15.117	4374	4378	4382	rBV3	756	852	0.10%	0.012%




Sum of corrected areas: 6847035

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
Data File : VV024251.D
Acq On : 30 Dec 2021 23:33
Operator : SY/MD
Sample : M5194-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

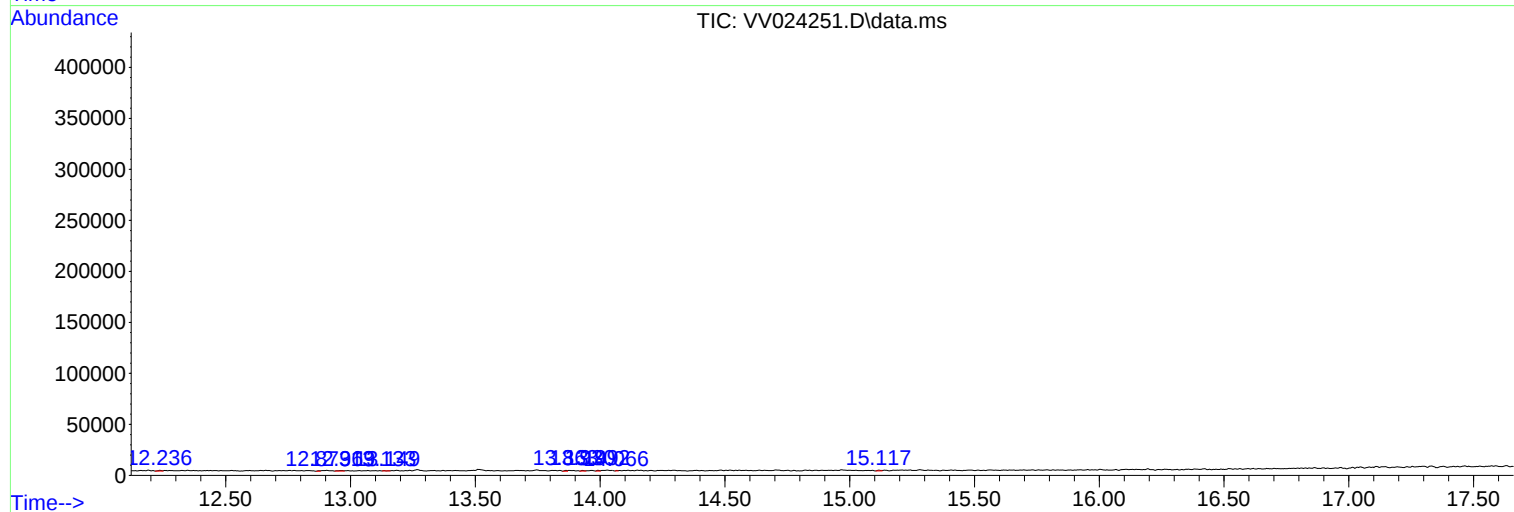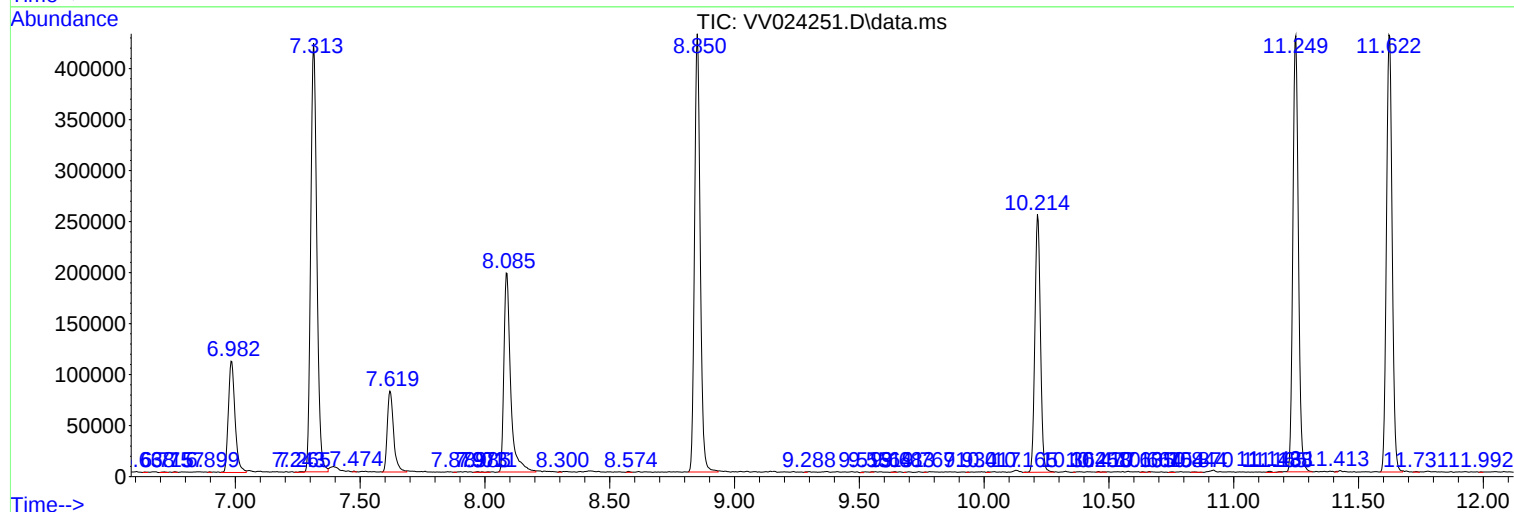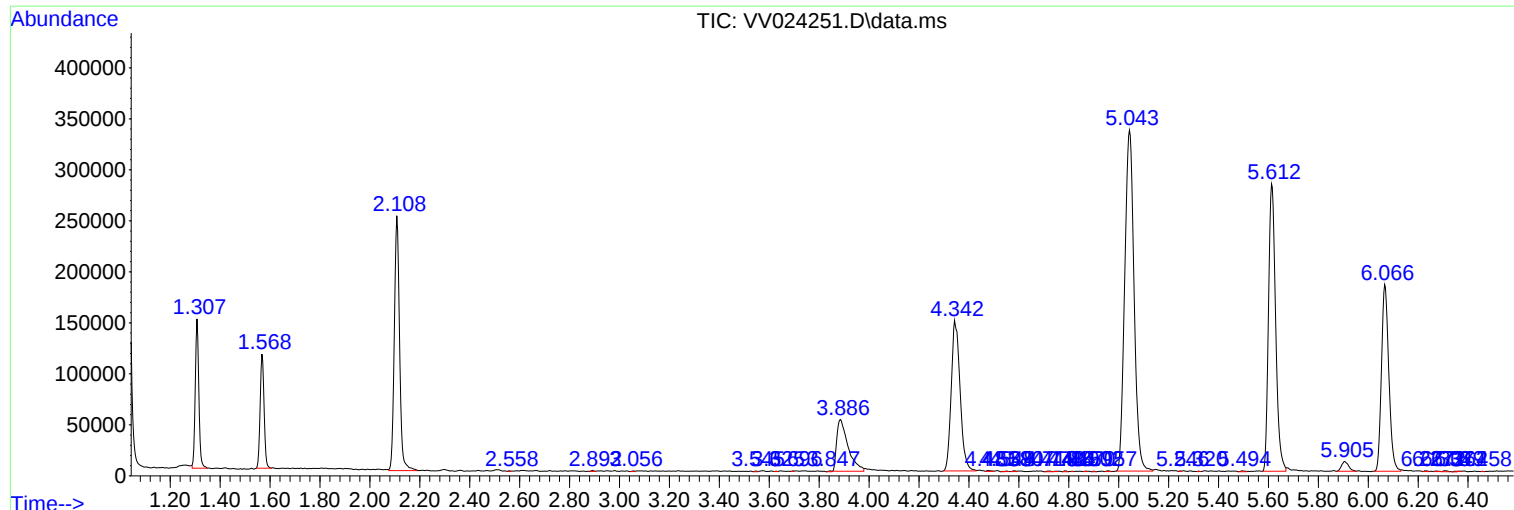

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
Data File : VV024251.D
Acq On : 30 Dec 2021 23:33
Operator : SY/MD
Sample : M5194-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
Data File : VV024251.D
Acq On : 30 Dec 2021 23:33
Operator : SY/MD
Sample : M5194-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc