

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW123121\
 Data File : VW024255.D
 Acq On : 31 Dec 2021 01:23
 Operator : SY/MD
 Sample : M5216-07
 Misc : 5.0ml/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

Signal : TIC: VW024255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	128995	133828	15.88%	2.087%
2	1.568	157	164	175	rBV	106783	117314	13.92%	1.830%
3	2.108	323	332	355	rVB	223993	325847	38.67%	5.082%
4	2.503	452	455	457	rBV3	1219	913	0.11%	0.014%
5	2.587	477	481	483	rBV	728	561	0.07%	0.009%
6	3.089	634	637	640	rVB2	556	304	0.04%	0.005%
7	3.114	641	645	647	rBV	514	436	0.05%	0.007%
8	3.423	738	741	744	rBV	310	212	0.03%	0.003%
9	3.455	748	751	755	rBV2	619	438	0.05%	0.007%
10	3.542	775	778	781	rBV	481	365	0.04%	0.006%
11	3.651	809	812	815	rBV2	729	455	0.05%	0.007%
12	3.712	828	831	834	rVB	637	356	0.04%	0.006%
13	3.886	874	885	923	rBV	52291	172238	20.44%	2.686%
14	4.346	1013	1028	1054	rBV	145460	359298	42.64%	5.604%
15	4.529	1082	1085	1087	rBV	299	225	0.03%	0.004%
16	4.561	1091	1095	1099	rVV2	540	576	0.07%	0.009%
17	4.677	1128	1131	1135	rVB	603	318	0.04%	0.005%
18	4.728	1143	1147	1148	rBV2	554	397	0.05%	0.006%
19	4.761	1154	1157	1158	rBV	426	263	0.03%	0.004%
20	4.834	1177	1180	1181	rBV	376	210	0.02%	0.003%
21	4.873	1188	1192	1195	rBV	408	325	0.04%	0.005%
22	4.950	1210	1216	1221	rBV2	698	1047	0.12%	0.016%
23	5.043	1229	1245	1274	rBV2	322004	842620	100.00%	13.143%
24	5.252	1305	1310	1313	rBV2	1088	1061	0.13%	0.017%
25	5.474	1377	1379	1382	rBV	419	260	0.03%	0.004%
26	5.558	1402	1405	1408	rBV2	391	262	0.03%	0.004%
27	5.616	1411	1423	1443	rBV	247579	497443	59.04%	7.759%
28	5.825	1485	1488	1490	rBV2	617	441	0.05%	0.007%
29	5.908	1504	1514	1531	rVB3	9241	19464	2.31%	0.304%
30	6.069	1550	1564	1582	rBV	183600	367364	43.60%	5.730%
31	6.214	1607	1609	1610	rBV	565	294	0.03%	0.005%
32	6.285	1629	1631	1636	rVB	472	331	0.04%	0.005%
33	6.310	1636	1639	1640	rBV	625	324	0.04%	0.005%
34	6.355	1650	1653	1658	rBV	462	466	0.06%	0.007%
35	6.461	1683	1686	1688	rBV	535	379	0.04%	0.006%
36	6.564	1714	1718	1722	rBV	605	481	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW123121\
 Data File : VW024255.D
 Acq On : 31 Dec 2021 01:23
 Operator : SY/MD
 Sample : M5216-07
 Misc : 5.0ml/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis

37	6.587	1722	1725	1728	rVB	370	219	0.03%	0.003%
38	6.609	1728	1732	1734	rBV	595	554	0.07%	0.009%
39	6.719	1764	1766	1771	rBV2	443	281	0.03%	0.004%
40	6.757	1774	1778	1781	rBV	506	448	0.05%	0.007%
41	6.889	1816	1819	1823	rVB2	628	430	0.05%	0.007%
42	6.915	1823	1827	1830	rBV	890	830	0.10%	0.013%
43	6.986	1838	1849	1869	rBV	104434	188028	22.31%	2.933%
44	7.243	1926	1929	1931	rBV	503	370	0.04%	0.006%
45	7.313	1940	1951	1971	rBV	387580	668477	79.33%	10.427%
46	7.551	2022	2025	2030	rBV3	548	586	0.07%	0.009%
47	7.619	2037	2046	2062	rBV2	78397	130142	15.44%	2.030%
48	8.088	2182	2192	2229	rBV	198793	372357	44.19%	5.808%
49	8.249	2239	2242	2244	rBV2	867	652	0.08%	0.010%
50	8.346	2268	2272	2274	rBV2	834	683	0.08%	0.011%
51	8.420	2289	2295	2302	rBV6	2532	3711	0.44%	0.058%
52	8.574	2340	2343	2345	rBV	338	198	0.02%	0.003%
53	8.850	2416	2429	2450	rBV	377085	602238	71.47%	9.393%
54	9.339	2578	2581	2584	rBV2	496	306	0.04%	0.005%
55	9.567	2649	2652	2656	rBV2	620	468	0.06%	0.007%
56	9.638	2672	2674	2677	rBV	473	371	0.04%	0.006%
57	9.870	2743	2746	2747	rBV	390	234	0.03%	0.004%
58	9.883	2747	2750	2753	rVV	530	459	0.05%	0.007%
59	10.214	2842	2853	2868	rBV	256330	392434	46.57%	6.121%
60	10.352	2892	2896	2900	rBV3	780	747	0.09%	0.012%
61	10.535	2950	2953	2954	rBV2	429	253	0.03%	0.004%
62	10.600	2971	2973	2980	rBV2	674	572	0.07%	0.009%
63	10.763	3022	3024	3027	rVB2	300	118	0.01%	0.002%
64	11.024	3103	3105	3107	rBV	253	143	0.02%	0.002%
65	11.249	3163	3175	3190	rBV	371210	566983	67.29%	8.843%
66	11.564	3271	3273	3276	rVB	543	224	0.03%	0.003%
67	11.622	3280	3291	3308	rVV	397437	624872	74.16%	9.746%
68	11.770	3335	3337	3341	rVB	649	405	0.05%	0.006%
69	12.024	3414	3416	3421	rVB2	781	657	0.08%	0.010%
70	12.050	3421	3424	3427	rBV	899	607	0.07%	0.009%
71	12.194	3466	3469	3472	rBV	508	441	0.05%	0.007%
72	12.574	3585	3587	3589	rBV	508	317	0.04%	0.005%
73	12.786	3650	3653	3654	rBV2	457	284	0.03%	0.004%
74	12.831	3665	3667	3671	rBV	495	330	0.04%	0.005%
75	12.943	3698	3702	3710	rVB	698	1005	0.12%	0.016%
76	12.979	3711	3713	3715	rBV	321	195	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
Data File : VV024255.D
Acq On : 31 Dec 2021 01:23
Operator : SY/MD
Sample : M5216-07
Misc : 5.0ml/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Title : VOC Analysis

77	13.866	3986	3989	3990	rBV	425	262	0.03%	0.004%
78	13.921	4002	4006	4010	rBV	540	599	0.07%	0.009%
79	14.037	4039	4042	4044	rBV2	503	315	0.04%	0.005%
80	15.461	4482	4485	4488	rVB	670	393	0.05%	0.006%




Sum of corrected areas: 6411314

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
Data File : VV024255.D
Acq On : 31 Dec 2021 01:23
Operator : SY/MD
Sample : M5216-07
Misc : 5.0ml/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

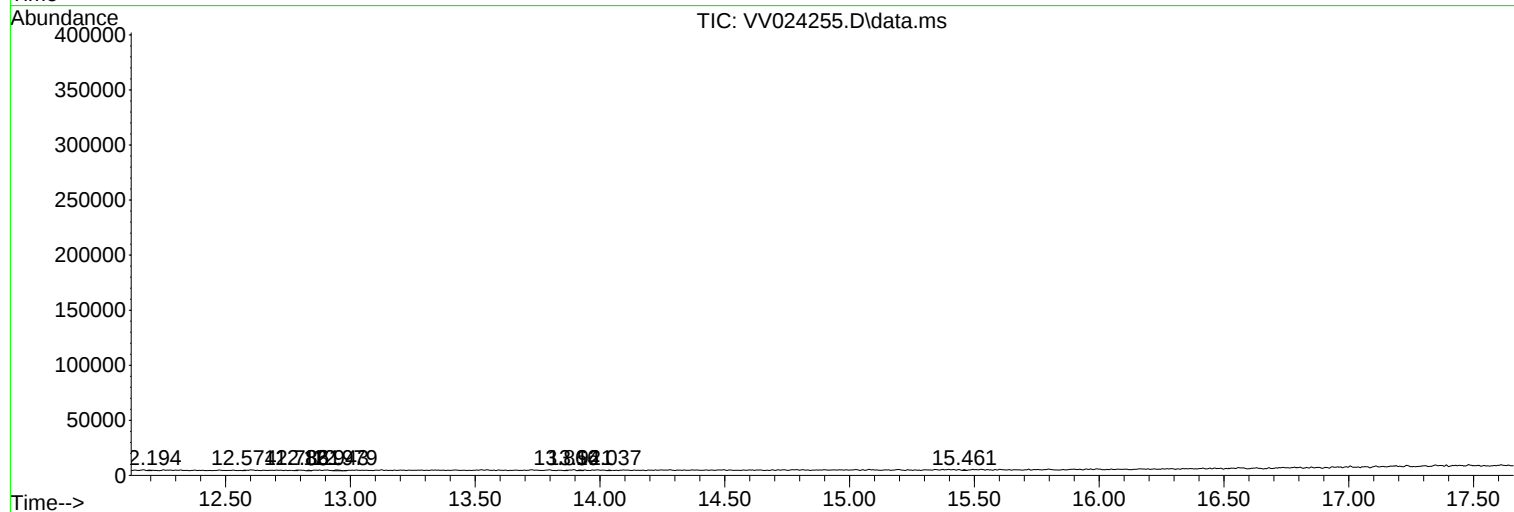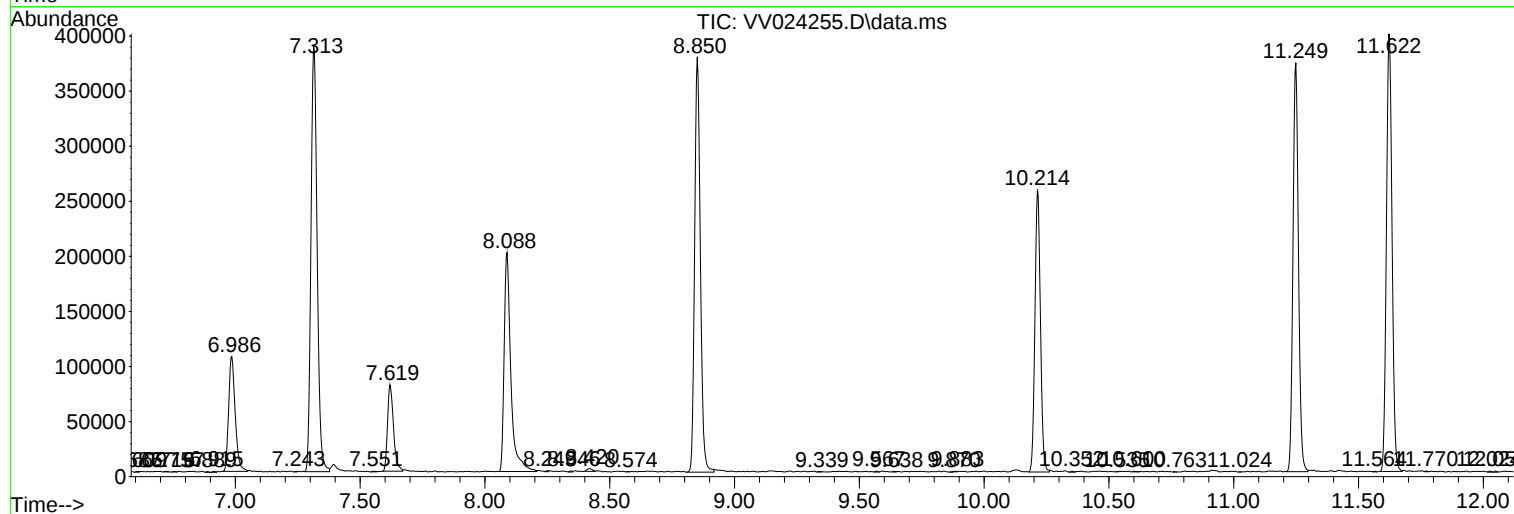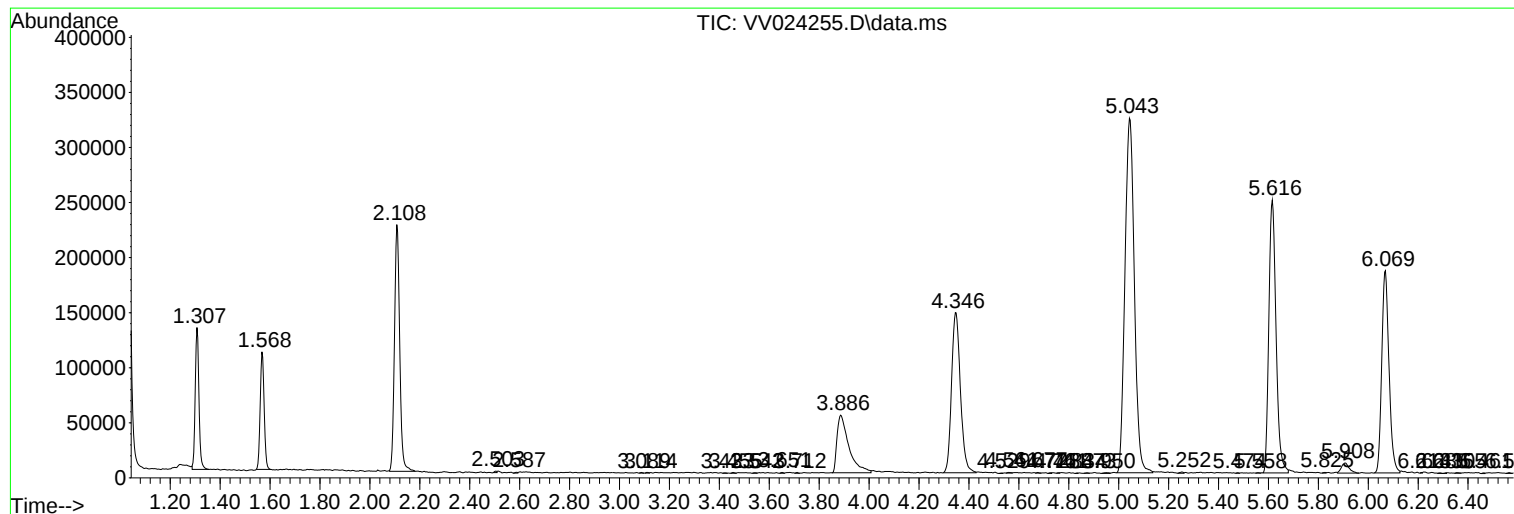

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
Data File : VV024255.D
Acq On : 31 Dec 2021 01:23
Operator : SY/MD
Sample : M5216-07
Misc : 5.0ml/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
Data File : VV024255.D
Acq On : 31 Dec 2021 01:23
Operator : SY/MD
Sample : M5216-07
Misc : 5.0ml/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc