
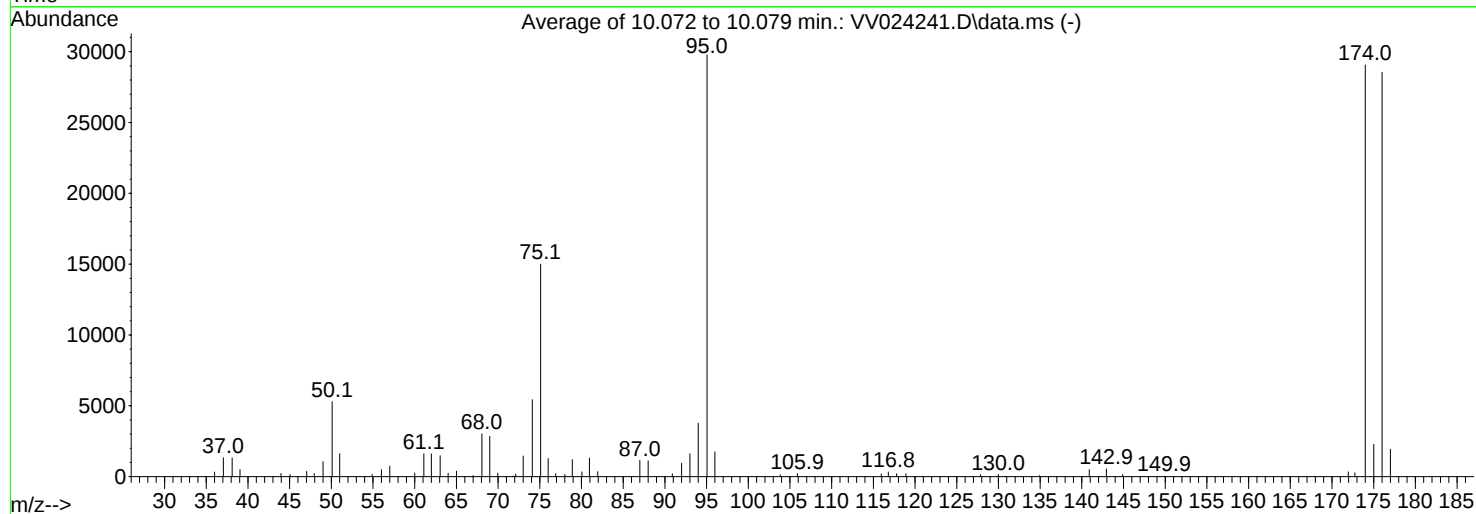


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV123121\
 Data File : VV024241.D
 Acq On : 30 Dec 2021 18:08
 Operator : SY/MD
 Sample : BFB250
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB250

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM123121WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 31 06:12:03 2021

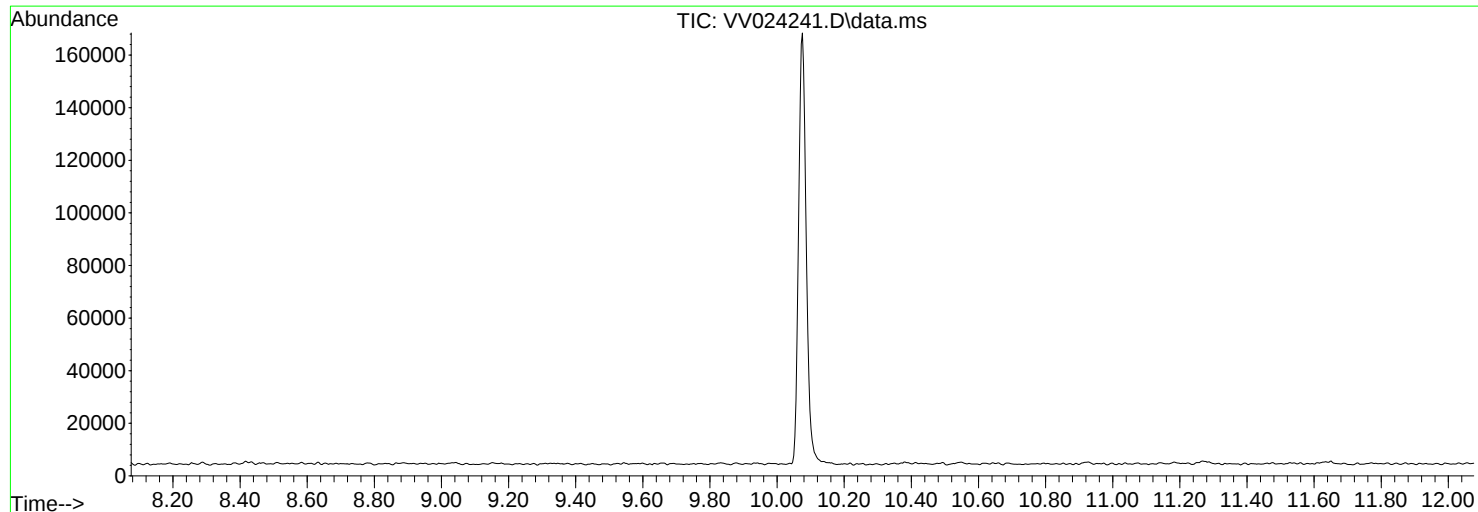

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	5296	PASS
75	95	30	80	50.4	15005	PASS
95	95	100	100	100.0	29776	PASS
96	95	5	9	5.9	1752	PASS
173	174	0.00	2	1.0	277	PASS
174	95	50	120	97.6	29064	PASS
175	174	5	9	7.8	2280	PASS
176	174	95	105	98.2	28547	PASS
177	176	5	10	6.8	1931	PASS

Scan 2799 (10.040 min): VV024241.D\data.ms
BFB250

m/z	Abundance
40.00	4526.0
43.90	118.0
45.20	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	329.0
37.00	1284.0
38.10	1345.0
39.10	481.0
40.00	4421.0
44.00	379.0
45.00	285.0
47.10	355.0
48.00	210.0
49.00	1045.0
50.10	5601.0
51.00	1803.0
54.90	204.0
56.00	512.0
57.00	712.0
60.00	290.0
61.10	1686.0
62.00	1729.0
63.00	1443.0
64.00	293.0
65.00	378.0
67.00	123.0
68.00	3096.0
69.00	2792.0
70.00	253.0
72.00	214.0
73.00	1432.0
74.10	5531.0
75.10	15763.0
76.00	1390.0
76.90	252.0
78.00	200.0
78.90	1282.0
80.10	328.0
80.90	1361.0
82.00	317.0
87.00	1142.0
88.00	1187.0
90.90	192.0
92.00	1046.0
93.00	1707.0
94.00	3741.0
95.10	29880.0
96.00	1767.0
103.80	134.0
105.90	225.0
116.00	209.0
116.80	333.0
117.80	217.0
118.90	196.0
127.80	134.0
130.00	150.0
140.90	462.0
142.90	552.0
145.00	163.0
171.90	338.0
172.70	269.0
174.00	28520.0
175.00	2398.0
176.00	28176.0
177.00	1947.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	333.0
37.10	1379.0
38.10	1388.0
39.00	508.0
40.00	4415.0
44.00	348.0
45.00	260.0
47.10	404.0
47.90	248.0
49.00	1102.0
50.10	5504.0
51.00	1666.0
54.90	163.0
56.00	501.0
57.00	753.0
60.00	250.0
61.10	1701.0
62.00	1648.0
63.10	1563.0
64.00	258.0
65.00	405.0
67.00	110.0
68.00	3087.0
69.00	2900.0
70.00	250.0
72.10	179.0
73.00	1520.0
74.10	5612.0
75.10	15537.0
76.00	1317.0
76.90	233.0
78.00	182.0
78.90	1216.0
80.00	346.0
80.90	1310.0
81.90	365.0
87.00	1189.0
88.00	1149.0
90.90	212.0
92.00	955.0
93.00	1695.0
94.00	3868.0
95.00	30704.0
96.00	1831.0
103.80	141.0
105.90	216.0
116.00	201.0
116.80	335.0
117.80	210.0
118.90	231.0
127.90	145.0
130.00	167.0
130.80	104.0
134.90	127.0
140.90	517.0
142.90	558.0
144.90	153.0
171.90	349.0
172.70	288.0
174.00	30120.0
175.00	2363.0
176.00	29632.0
177.00	1978.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	326.0
37.10	1320.0
38.10	1233.0
39.00	509.0
40.00	4432.0
44.00	296.0
45.00	244.0
47.00	373.0
47.90	213.0
49.00	1049.0
50.10	4783.0
51.00	1363.0
54.90	115.0
56.00	472.0
57.00	760.0
60.00	228.0
61.10	1474.0
62.00	1425.0
63.10	1437.0
64.00	207.0
65.00	367.0
68.10	2869.0
69.00	2837.0
69.90	239.0
71.80	142.0
72.20	149.0
73.00	1423.0
74.10	5144.0
75.10	13716.0
76.00	1115.0
76.90	174.0
78.00	109.0
78.90	1107.0
80.00	351.0
81.00	1250.0
81.90	367.0
87.00	1109.0
88.00	1020.0
90.90	221.0
92.00	830.0
93.00	1433.0
94.00	3707.0
95.00	28744.0
96.00	1657.0
103.90	129.0
105.90	197.0
115.90	172.0
116.80	323.0
117.80	178.0
118.90	207.0
127.90	138.0
130.00	152.0
134.90	110.0
140.90	501.0
143.00	504.0
144.80	134.0
149.90	106.0
172.00	328.0
172.80	274.0
174.00	28552.0
175.00	2079.0
176.00	27832.0
177.00	1867.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250