

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011624\
 Data File : VW033678.D
 Acq On : 16 Jan 2024 18:08
 Operator : SY/MD
 Sample : P1131-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B02

Quant Time: Jan 17 00:14:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 17 00:08:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	105547	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	98928	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	49500	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	21780	3.774	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.400%
7) Chloroethane-d5	1.536	69	21639	4.227	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.600%
11) 1,1-Dichloroethene-d2	2.063	65	10877	4.182	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.600%
20) 2-Butanone-d5	3.809	46	67056	47.519	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.040%
24) Chloroform-d	4.252	84	57719	4.624	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
26) 1,2-Dichloroethane-d4	4.947	65	27903	4.986	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	4.963	84	106535	4.463	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	5.992	67	34669	4.356	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.200%
41) Toluene-d8	7.246	98	95257	4.470	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.400%
43) trans-1,3-Dichloroprop...	7.561	79	11967	4.350	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.000%
46) 2-Hexanone-d5	8.027	63	50369	46.629	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.260%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	22580	4.856	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	11.561	152	36860	4.850	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.000%
Target Compounds						
					Qvalue	
25) Chloroform	4.281	83	9630	0.628	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033678.D
Acq On : 16 Jan 2024 18:08
Operator : SY/MD
Sample : P1131-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B02

Quant Time: Jan 17 00:14:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 17 00:08:33 2024
Response via : Initial Calibration

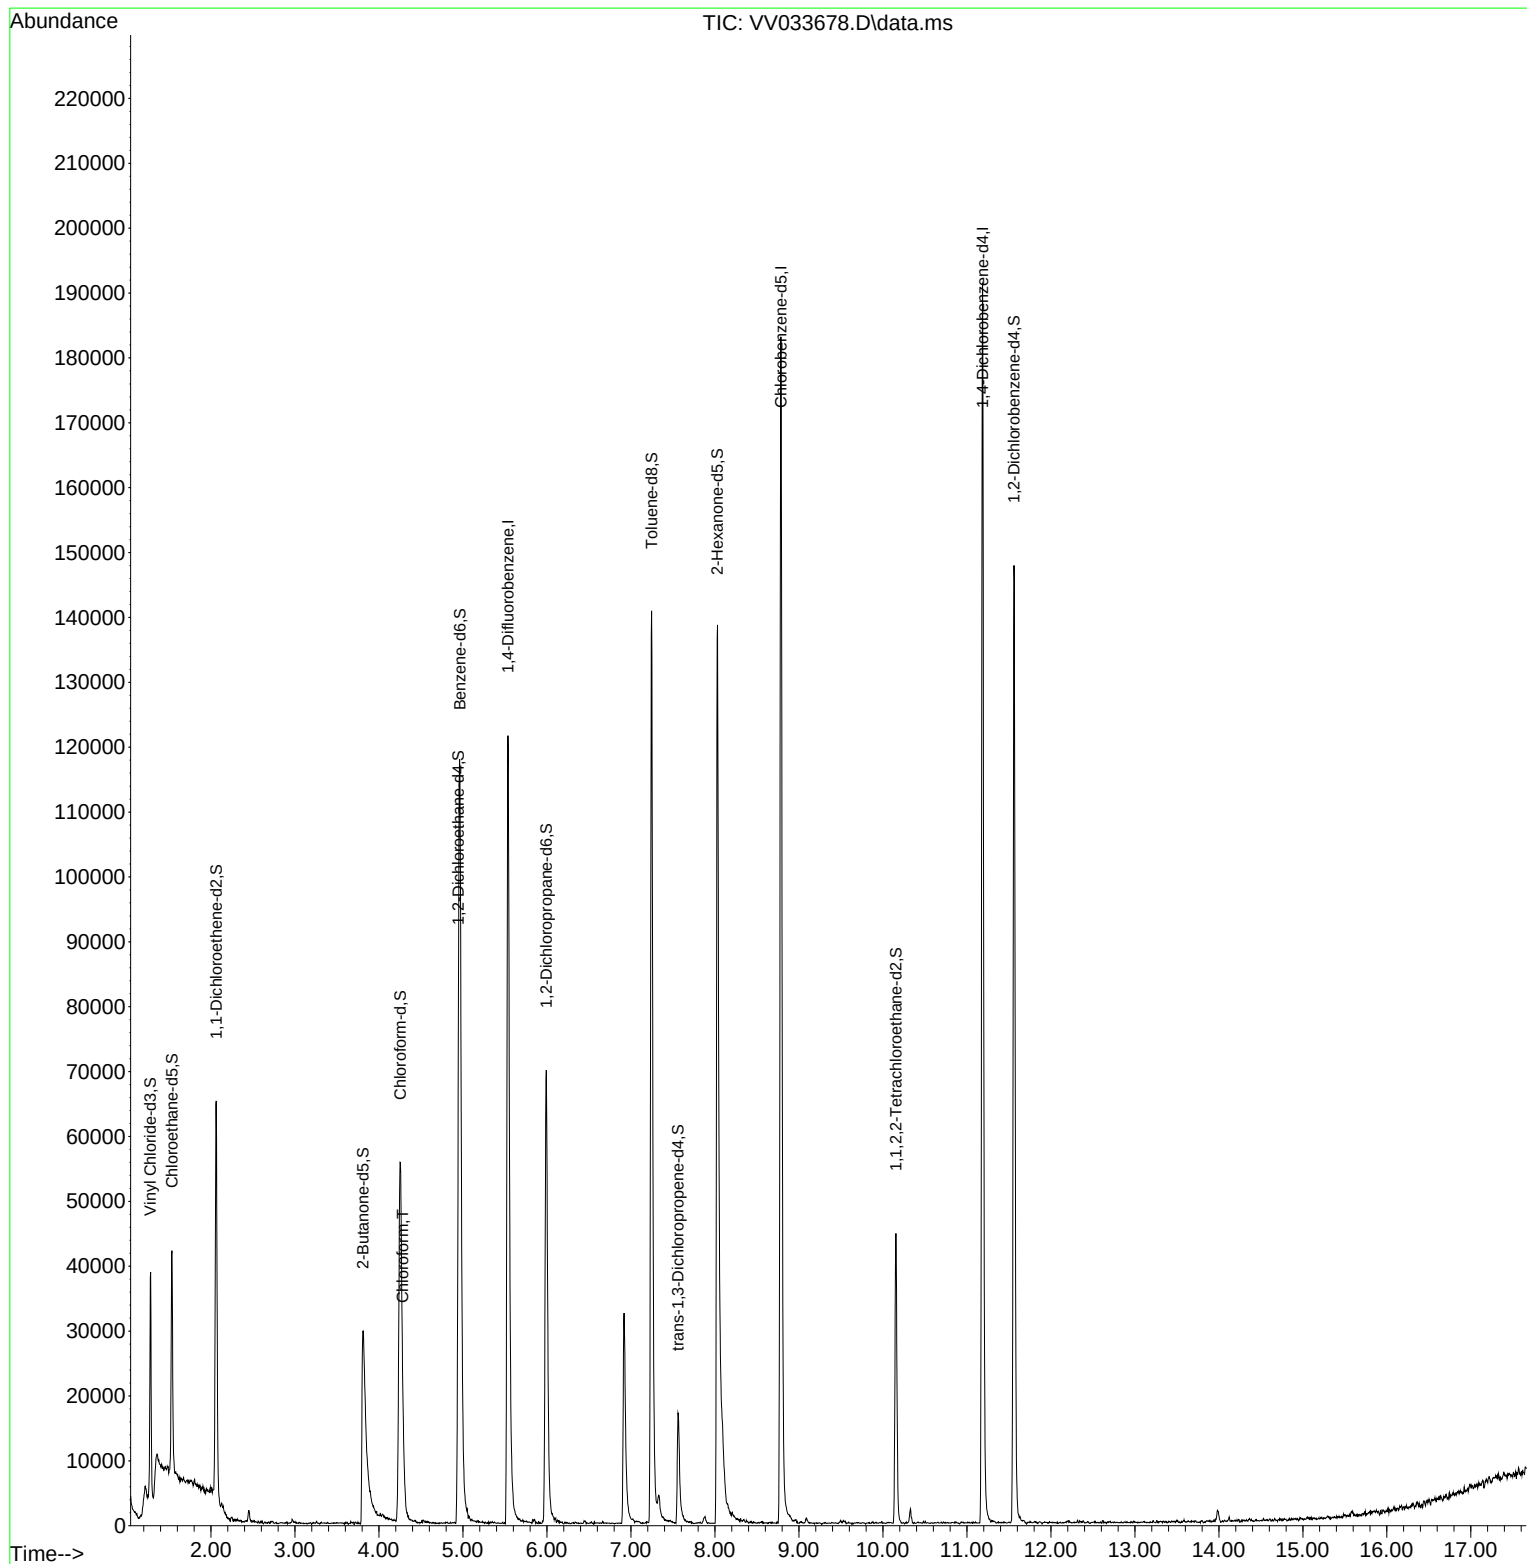

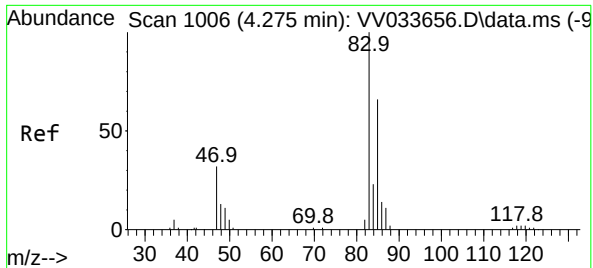

#25
 Chloroform
 Concen: 0.628 ug/L
 RT: 4.281 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV033678.D
 Acq: 16 Jan 2024 18:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B02

Tgt Ion: 83 Resp: 9630
 Ion Ratio Lower Upper
 83 100
 85 62.6 45.1 83.9

