

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033681.D
 Acq On : 16 Jan 2024 19:20
 Operator : SY/MD
 Sample : P1131-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B00

Quant Time: Jan 17 00:15:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 17 00:08:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	103941	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	97137	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	49819	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	20321	3.575	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.600%
7) Chloroethane-d5	1.535	69	20984	4.163	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.200%
11) 1,1-Dichloroethene-d2	2.063	65	10503	4.100	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.000%
20) 2-Butanone-d5	3.812	46	67574	48.626	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.260%
24) Chloroform-d	4.255	84	55424	4.509	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.200%
26) 1,2-Dichloroethane-d4	4.950	65	27498	4.990	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	4.963	84	104828	4.473	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
36) 1,2-Dichloropropane-d6	5.992	67	34390	4.401	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.000%
41) Toluene-d8	7.246	98	91934	4.394	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
43) trans-1,3-Dichloroprop...	7.561	79	11302	4.184	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.030	63	51513	48.568	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.140%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	22780	4.989	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	36370	4.755	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.000%
Target Compounds					Qvalue	
25) Chloroform	4.288	83	10064	0.666	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033681.D
Acq On : 16 Jan 2024 19:20
Operator : SY/MD
Sample : P1131-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Time: Jan 17 00:15:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 17 00:08:33 2024
Response via : Initial Calibration

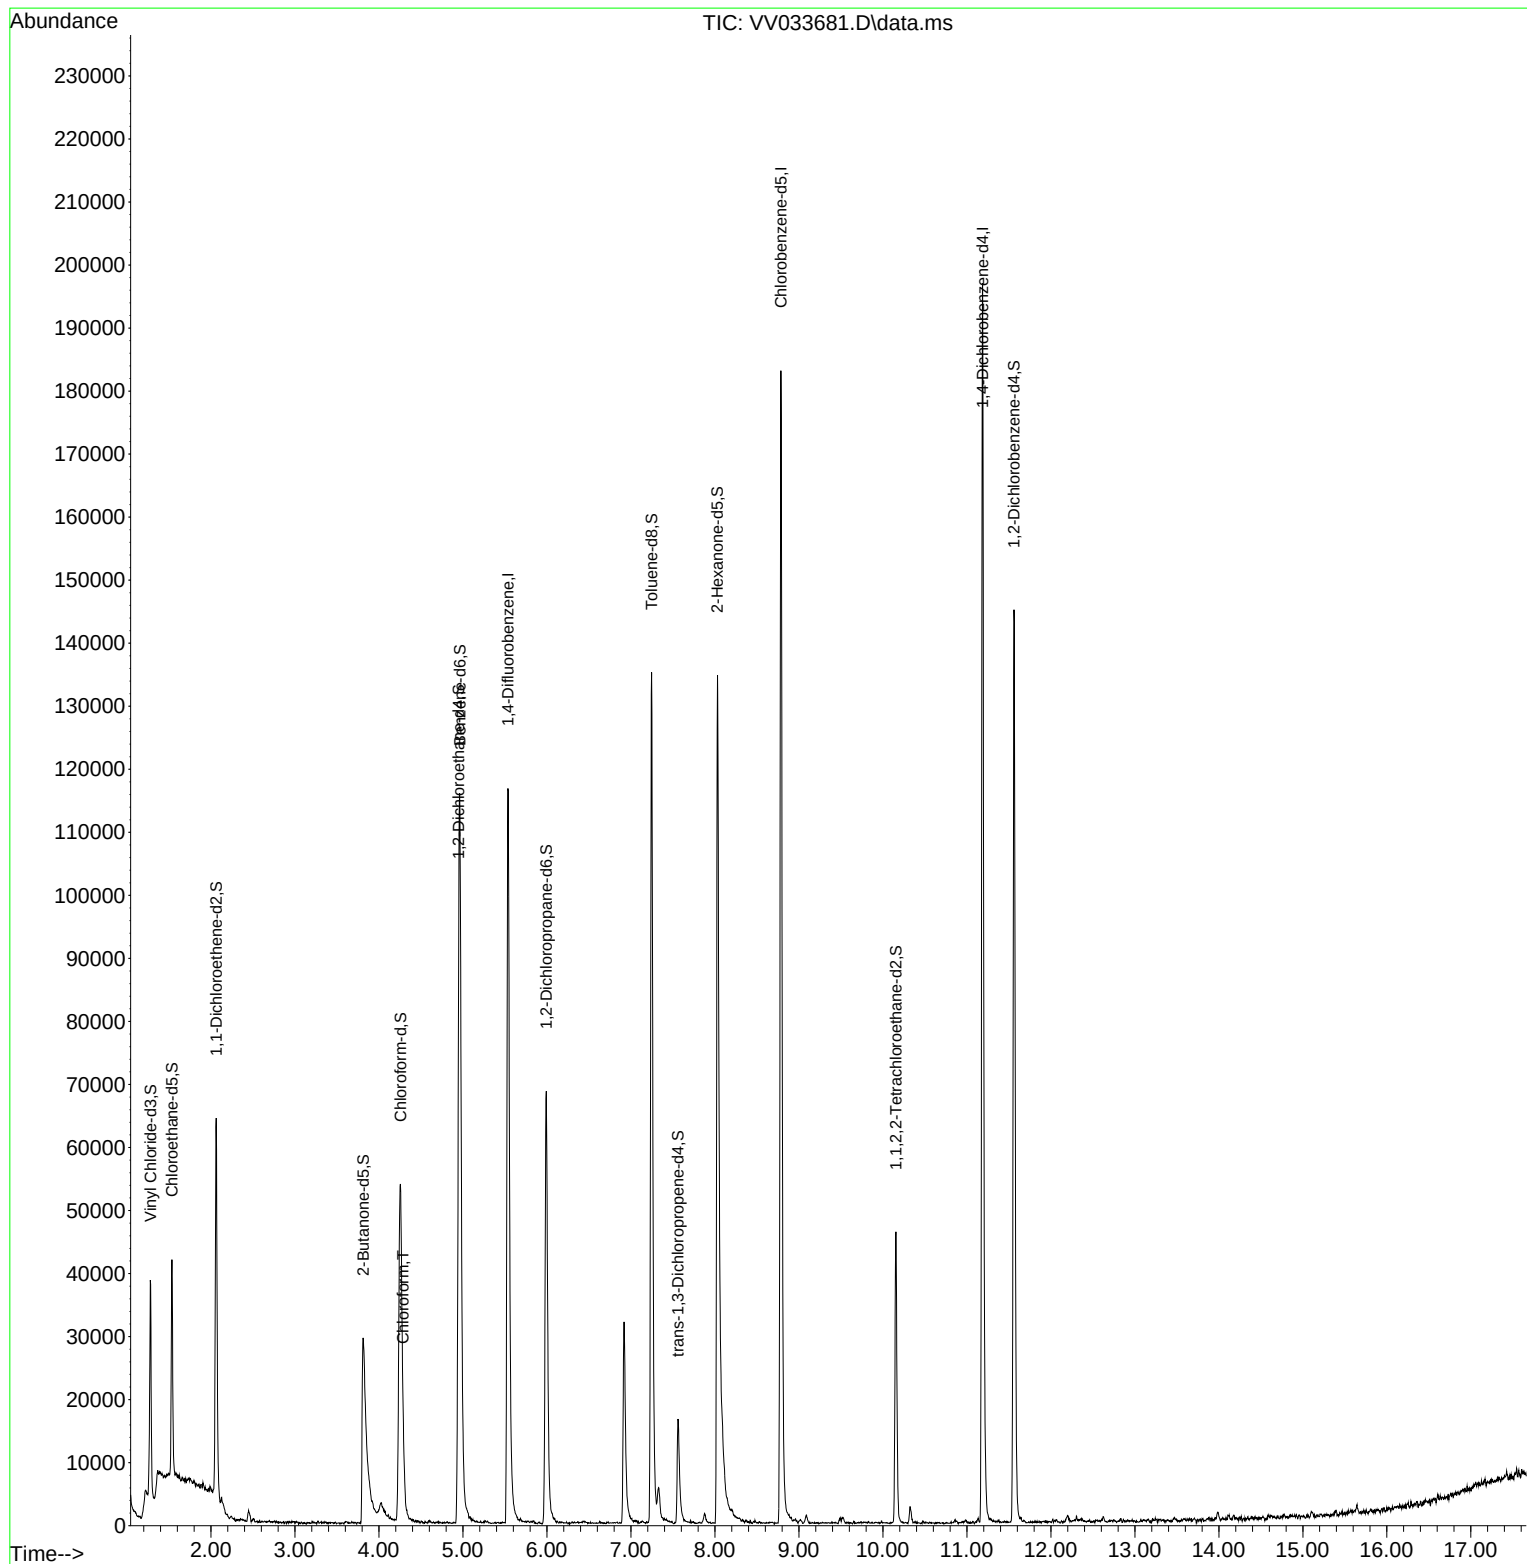

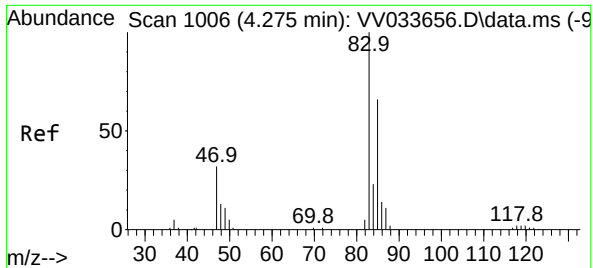

#25
 Chloroform
 Concen: 0.666 ug/L
 RT: 4.288 min Scan# 10
 Delta R.T. 0.013 min
 Lab File: VV033681.D
 Acq: 16 Jan 2024 19:20

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B00

Tgt Ion: 83 Resp: 10064
 Ion Ratio Lower Upper
 83 100
 85 62.5 45.1 83.9

