

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011624\
 Data File : VW033697.D
 Acq On : 17 Jan 2024 02:08
 Operator : SY/MD
 Sample : P1143-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B07

Quant Time: Jan 17 03:33:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 17 01:35:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	105810	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	96688	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	50664	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	19840	3.429	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.600%
7) Chloroethane-d5	1.536	69	20672	4.028	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.600%
11) 1,1-Dichloroethene-d2	2.060	65	10225	3.921	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.400%
20) 2-Butanone-d5	3.809	46	67150	47.467	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.940%
24) Chloroform-d	4.256	84	57270	4.577	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	4.947	65	27619	4.923	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	4.963	84	104408	4.475	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	5.992	67	34548	4.442	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.800%
41) Toluene-d8	7.246	98	94021	4.514	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.200%
43) trans-1,3-Dichloroprop...	7.561	79	11931	4.437	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.800%
46) 2-Hexanone-d5	8.027	63	50979	48.288	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.580%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	22678	4.990	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	37502	4.821	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds						
					Qvalue	
25) Chloroform	4.281	83	10192	0.663	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033697.D
Acq On : 17 Jan 2024 02:08
Operator : SY/MD
Sample : P1143-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B07

Quant Time: Jan 17 03:33:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 17 01:35:32 2024
Response via : Initial Calibration

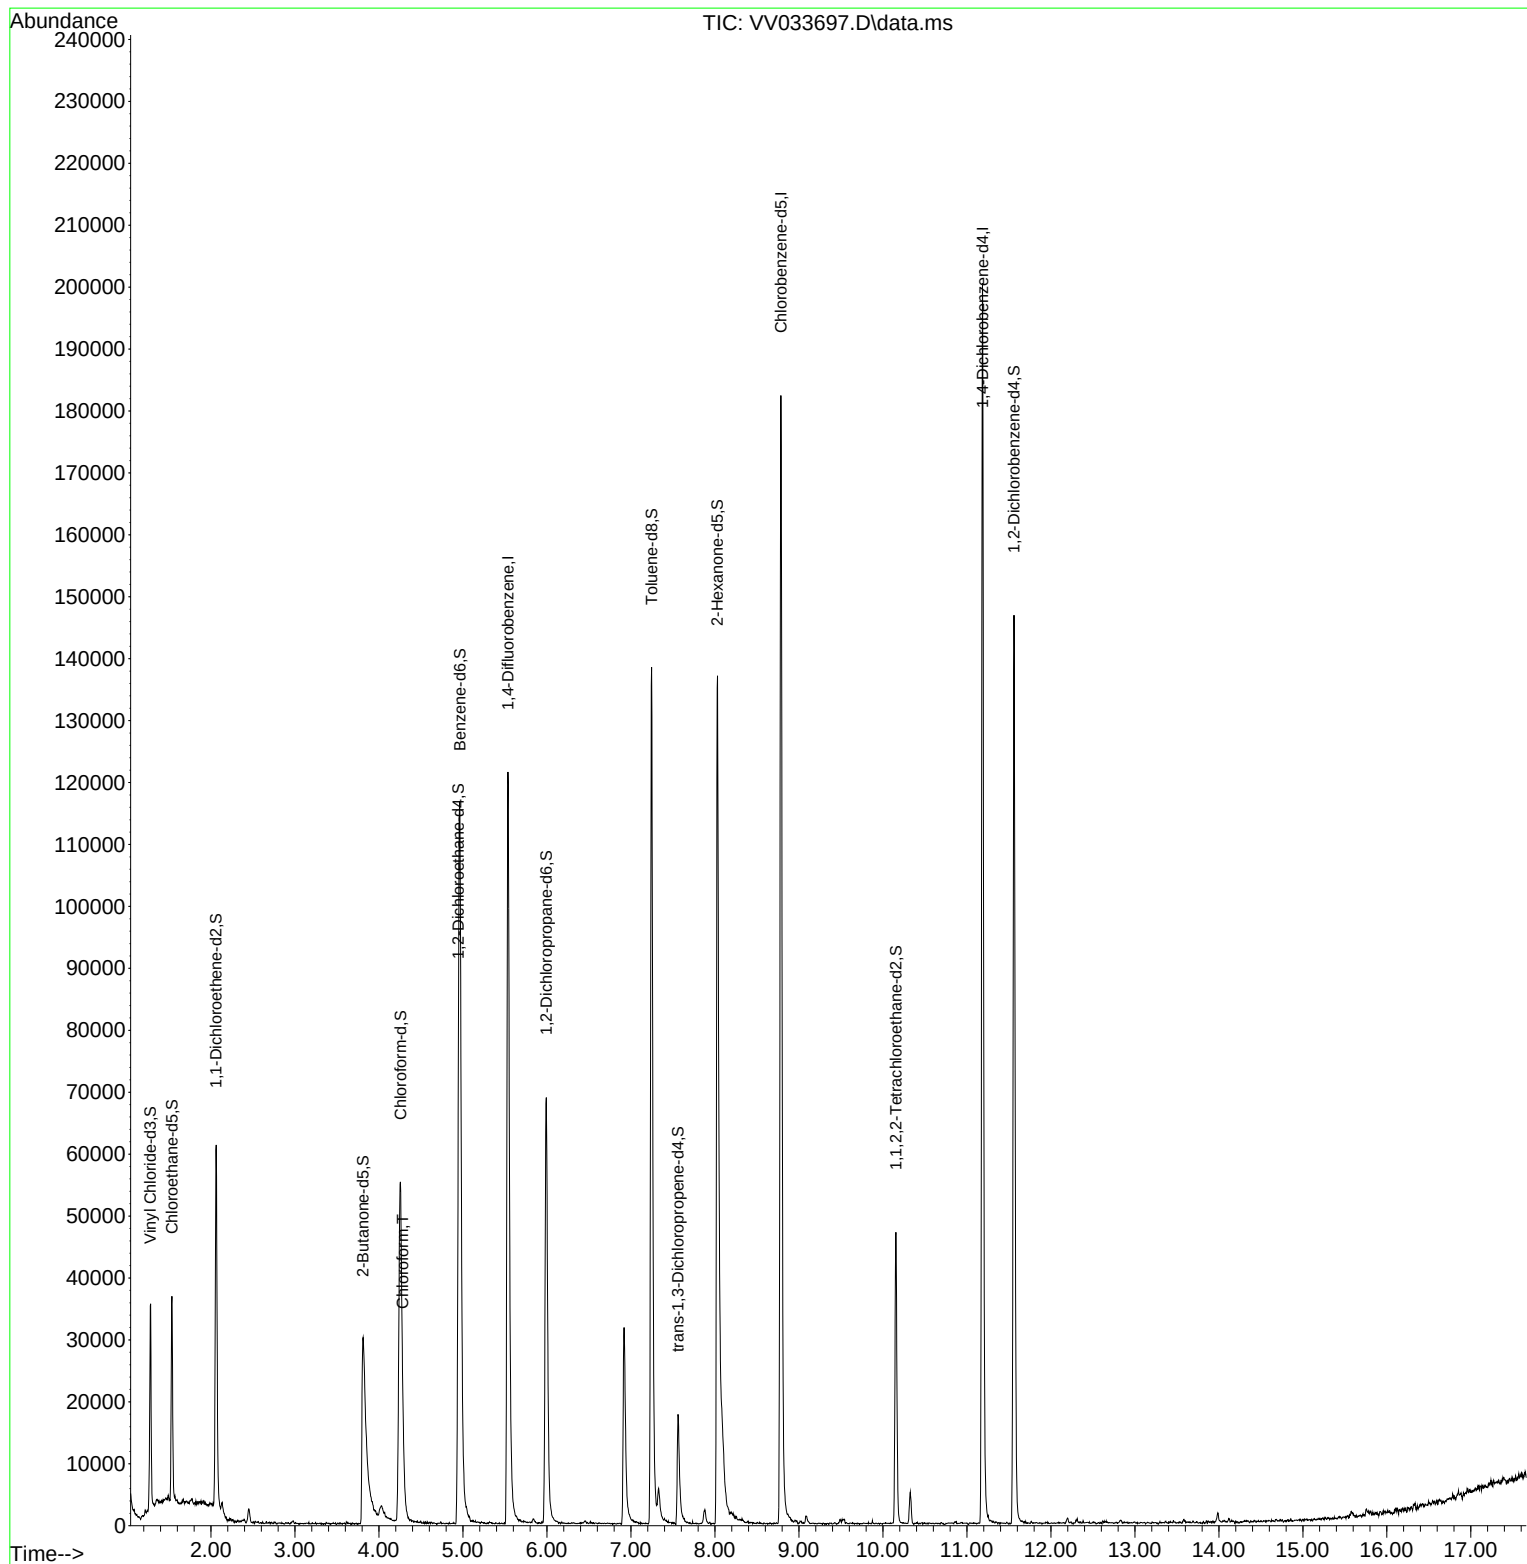

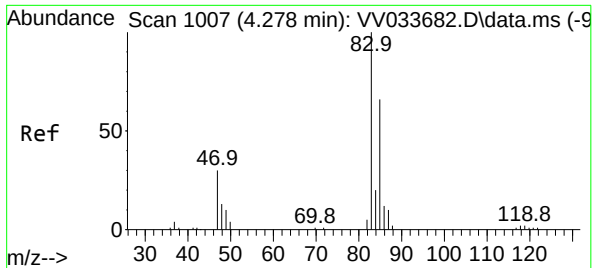

#25
 Chloroform
 Concen: 0.663 ug/L
 RT: 4.281 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV033697.D
 Acq: 17 Jan 2024 02:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B07

Tgt Ion: 83 Resp: 10192
 Ion Ratio Lower Upper
 83 100
 85 67.9 45.1 83.9

