

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033702.D
 Acq On : 17 Jan 2024 04:07
 Operator : SY/MD
 Sample : P1143-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B65

Quant Time: Jan 17 04:32:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 17 01:35:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	111456	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	104842	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	54460	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	20171	3.310	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.200%
7) Chloroethane-d5	1.535	69	21213	3.924	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.400%
11) 1,1-Dichloroethene-d2	2.063	65	10321	3.758	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.200%
20) 2-Butanone-d5	3.809	46	67949	45.599	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.200%
24) Chloroform-d	4.252	84	57986	4.400	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
26) 1,2-Dichloroethane-d4	4.947	65	28038	4.745	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	4.963	84	105031	4.152	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
36) 1,2-Dichloropropane-d6	5.992	67	34785	4.124	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.400%
41) Toluene-d8	7.246	98	92303	4.087	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.800%
43) trans-1,3-Dichloroprop...	7.561	79	11627	3.988	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.800%
46) 2-Hexanone-d5	8.030	63	52887	46.199	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.400%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	22991	4.665	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	37414	4.474	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.400%
Target Compounds					Qvalue	
25) Chloroform	4.278	83	11531	0.712	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033702.D
Acq On : 17 Jan 2024 04:07
Operator : SY/MD
Sample : P1143-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B65

Quant Time: Jan 17 04:32:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 17 01:35:32 2024
Response via : Initial Calibration

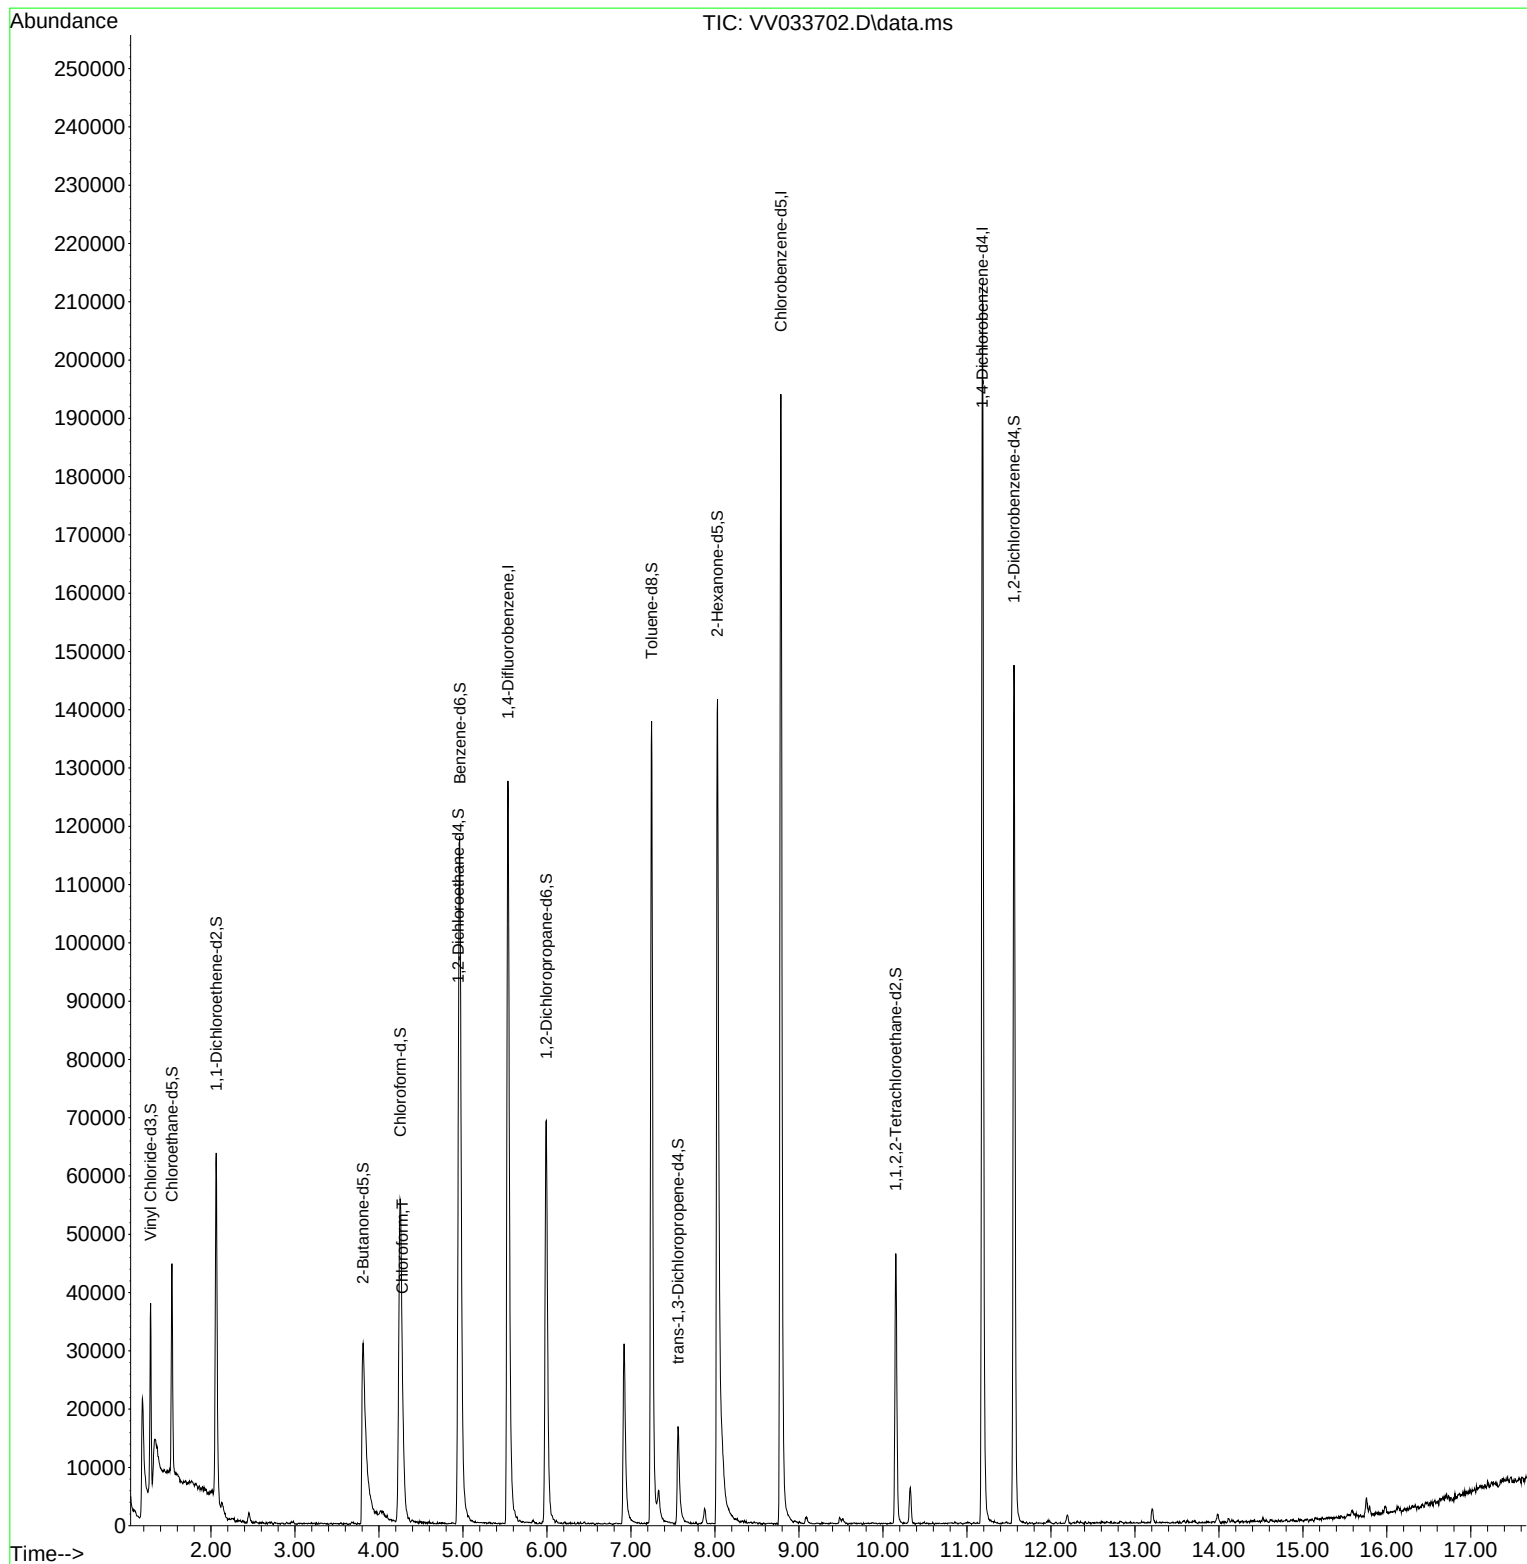

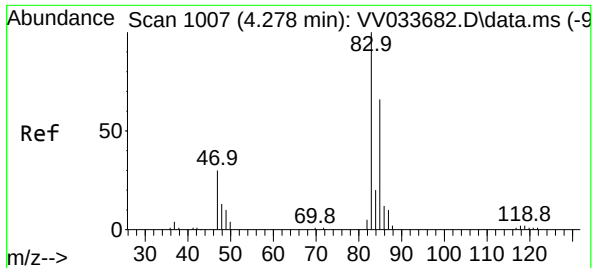

#25
 Chloroform
 Concen: 0.712 ug/L
 RT: 4.278 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: VV033702.D
 Acq: 17 Jan 2024 04:07

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B65

Tgt Ion: 83 Resp: 11531
 Ion Ratio Lower Upper
 83 100
 85 60.3 45.1 83.9

