

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW011624\
 Data File : VW033703.D
 Acq On : 17 Jan 2024 04:30
 Operator : SY/MD
 Sample : P1143-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B66

Quant Time: Jan 17 04:56:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 17 01:35:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	109530	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	100361	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	52230	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	20137	3.362	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.200%
7) Chloroethane-d5	1.536	69	21046	3.962	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.200%
11) 1,1-Dichloroethene-d2	2.063	65	10426	3.863	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.200%
20) 2-Butanone-d5	3.812	46	68366	46.685	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.380%
24) Chloroform-d	4.252	84	56799	4.385	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	4.947	65	27603	4.753	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.000%
32) Benzene-d6	4.963	84	104822	4.329	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%
36) 1,2-Dichloropropane-d6	5.992	67	34143	4.229	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.600%
41) Toluene-d8	7.246	98	91481	4.232	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.600%
43) trans-1,3-Dichloroprop...	7.561	79	11685	4.186	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.800%
46) 2-Hexanone-d5	8.030	63	51864	47.328	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.660%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	23055	4.887	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.800%
66) 1,2-Dichlorobenzene-d4	11.564	152	37161	4.634	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.600%
Target Compounds						
					Qvalue	
25) Chloroform	4.278	83	10621	0.667	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033703.D
Acq On : 17 Jan 2024 04:30
Operator : SY/MD
Sample : P1143-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B66

Quant Time: Jan 17 04:56:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 17 01:35:32 2024
Response via : Initial Calibration

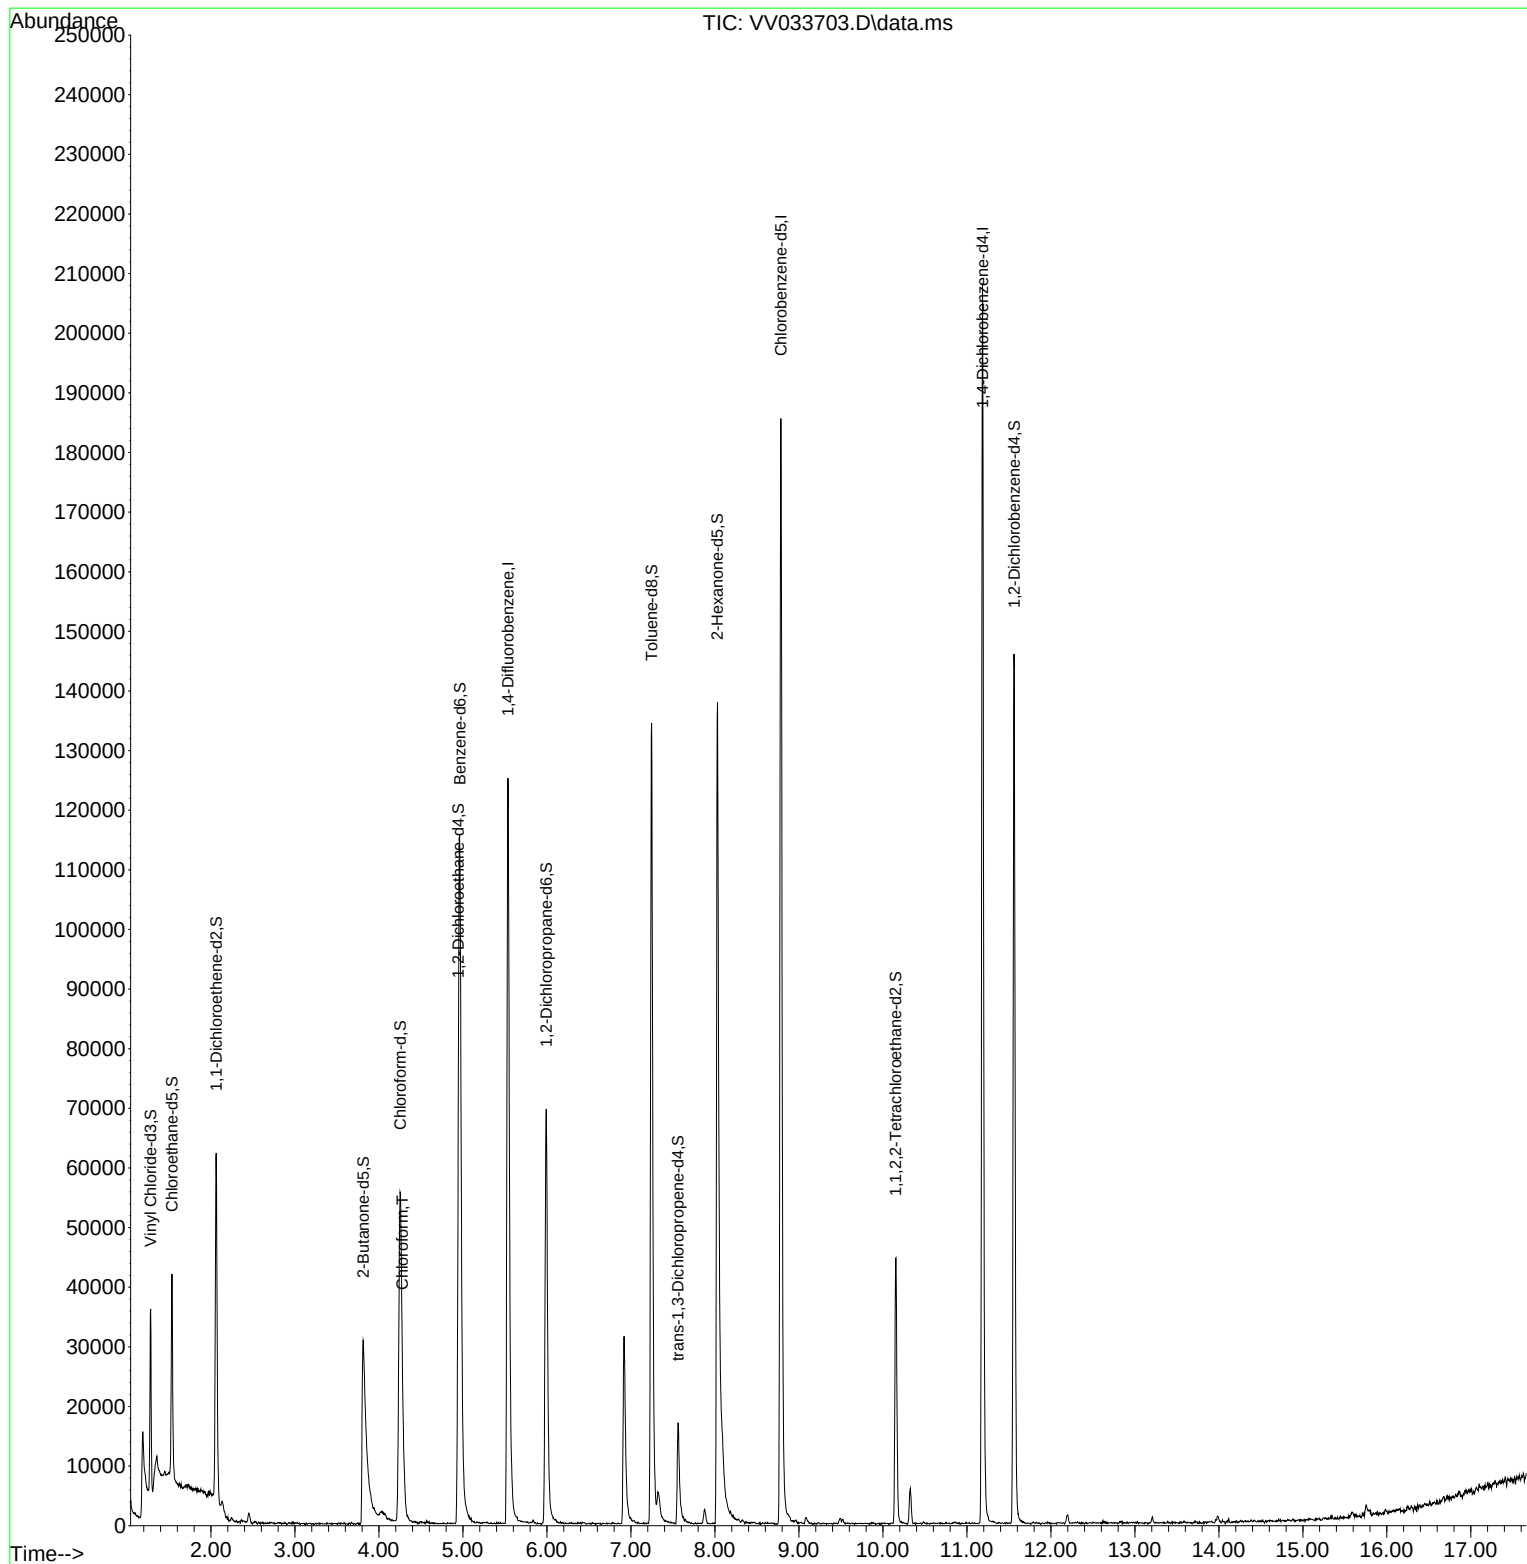

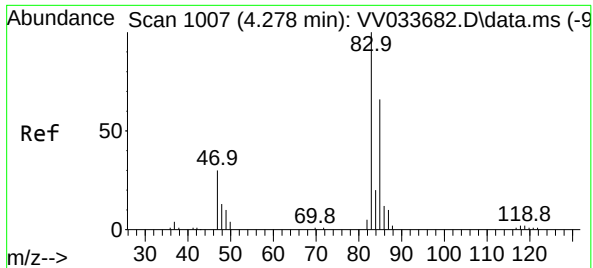

#25
 Chloroform
 Concen: 0.667 ug/L
 RT: 4.278 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: VV033703.D
 Acq: 17 Jan 2024 04:30

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B66

Tgt Ion: 83 Resp: 10621
 Ion Ratio Lower Upper
 83 100
 85 69.6 45.1 83.9

