

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033666.D
 Acq On : 16 Jan 2024 13:24
 Operator : SY/MD
 Sample : P1062-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH265

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rBV	36324	37556	11.49%	1.209%
2	1.536	146	154	163	rBV	36552	43346	13.26%	1.396%
3	2.063	309	318	331	rVB	64281	95892	29.34%	3.087%
4	2.368	367	413	416	rBV2	31979	151751	46.43%	4.886%
5	2.516	450	459	489	rVB	60280	125281	38.33%	4.033%
6	3.819	855	864	900	rBV2	27492	109052	33.36%	3.511%
7	4.253	983	999	1025	rBV	55624	143738	43.97%	4.628%
8	4.960	1201	1219	1245	rBV3	124874	318092	97.32%	10.241%
9	5.535	1387	1398	1434	rBV	127981	268968	82.29%	8.659%
10	5.992	1527	1540	1566	rBV2	72865	156351	47.83%	5.034%
11	6.918	1817	1828	1853	rBV	32443	66165	20.24%	2.130%
12	7.246	1917	1930	1954	rBV	145757	266186	81.44%	8.570%
13	7.561	2020	2028	2048	rBV2	17369	35043	10.72%	1.128%
14	8.031	2165	2174	2213	rBV	140406	315312	96.47%	10.152%
15	8.786	2399	2409	2436	rBV	189655	322761	98.74%	10.391%
16	10.156	2823	2835	2852	rBV	46434	75631	23.14%	2.435%
17	10.326	2880	2888	2897	rVB3	4644	7362	2.25%	0.237%
18	11.188	3144	3156	3179	rBV	205831	326866	100.00%	10.524%
19	11.561	3261	3272	3294	rBV	147974	240696	73.64%	7.749%




Sum of corrected areas: 3106049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033666.D
Acq On : 16 Jan 2024 13:24
Operator : SY/MD
Sample : P1062-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

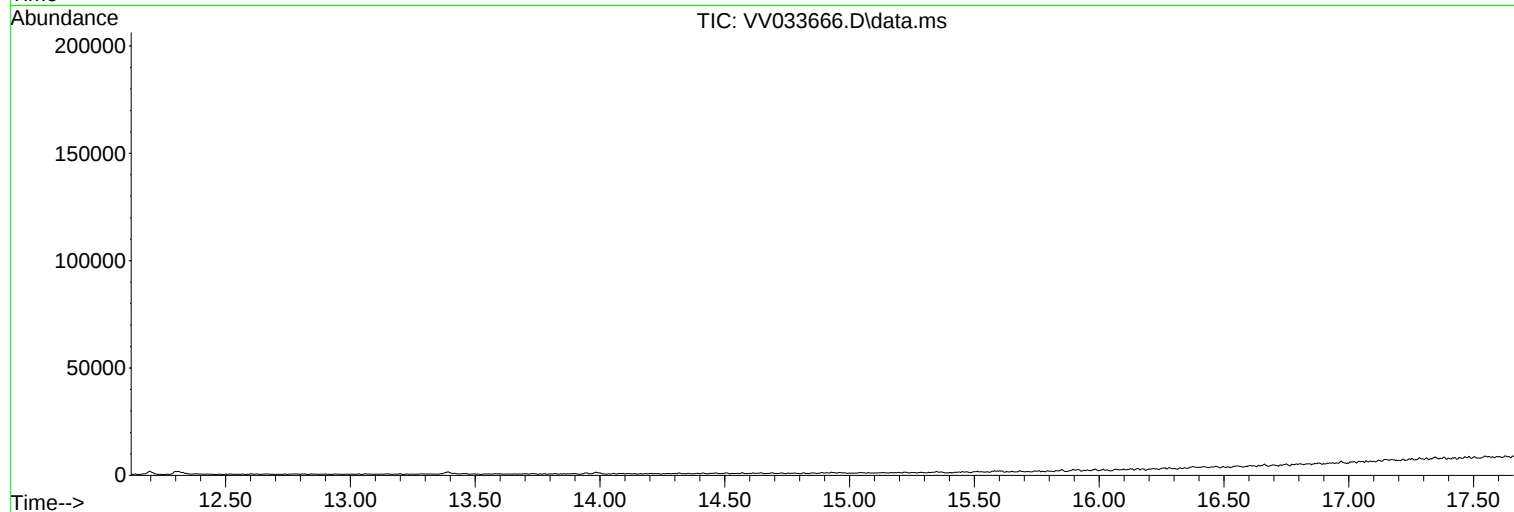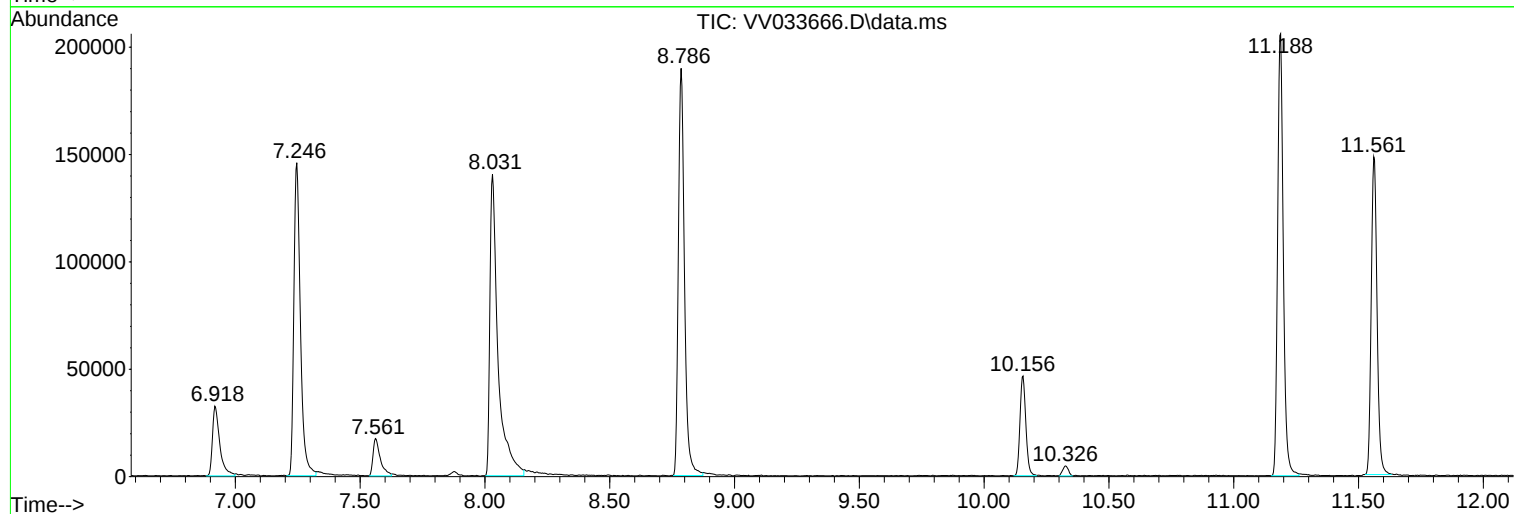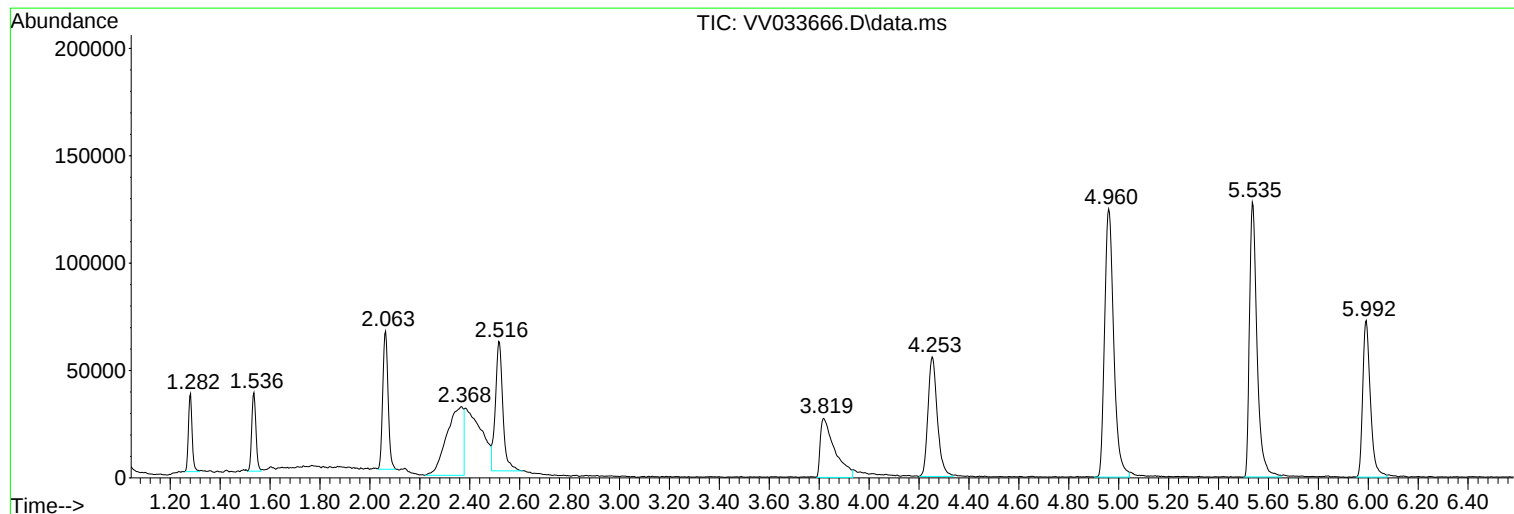

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033666.D
Acq On : 16 Jan 2024 13:24
Operator : SY/MD
Sample : P1062-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH265










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.368	2.82 ug/L	151751	1,4-Difluorobenzene	5.535

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	83
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	83
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	83
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

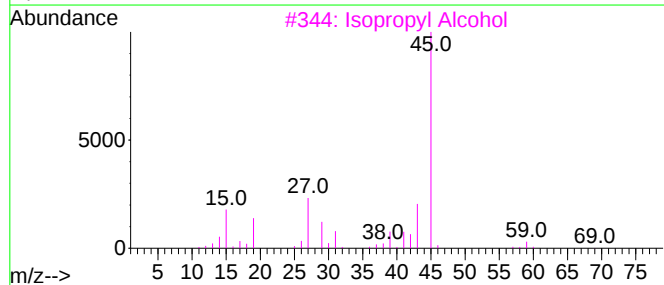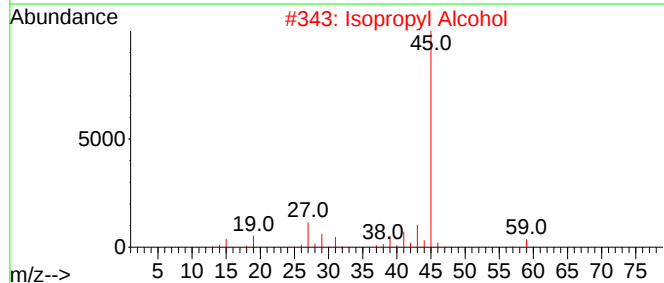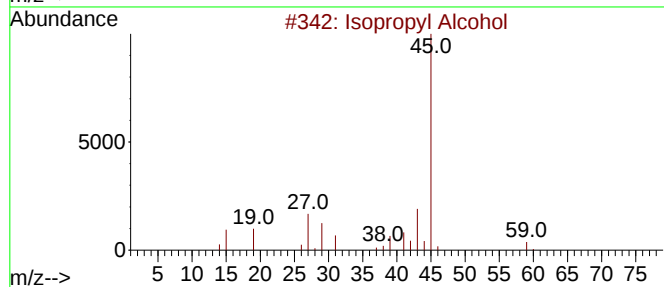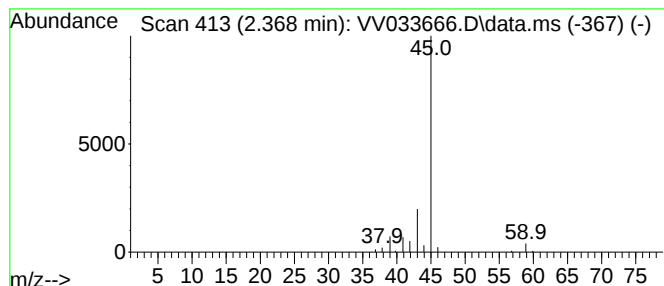

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033666.D
Acq On : 16 Jan 2024 13:24
Operator : SY/MD
Sample : P1062-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH265










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic2.516 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.516	2.33 ug/L	125281	1,4-Difluorobenzene	5.535

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentane	70	C5H10	000287-92-3	90
2			Cyclobutane, methyl-	70	C5H10	000598-61-8	86
3			Cyclopentane	70	C5H10	000287-92-3	86
4			1-Pentene	70	C5H10	000109-67-1	83
5			Cyclopentane	70	C5H10	000287-92-3	72

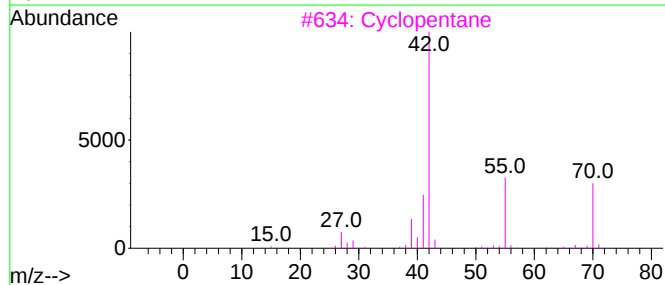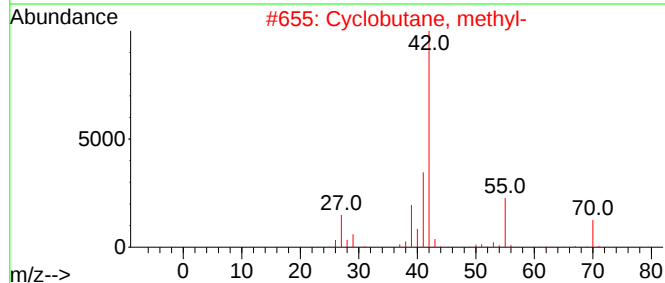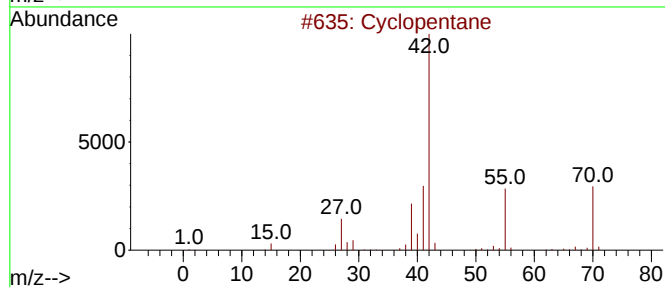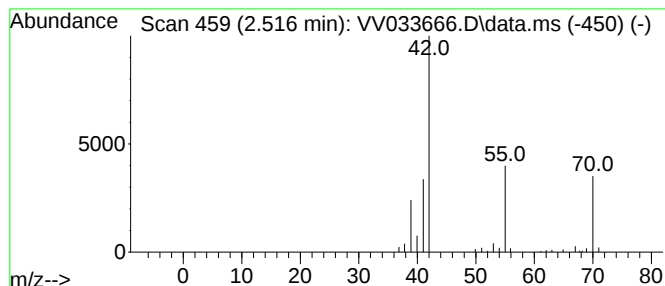

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033666.D
Acq On : 16 Jan 2024 13:24
Operator : SY/MD
Sample : P1062-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.368	2.8	ug/L	151751	1	5.535	268968	5.0
(DEL) Alkane: C...	2.516	2.3	ug/L	125281	1	5.535	268968	5.0