

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033667.D
 Acq On : 16 Jan 2024 13:48
 Operator : SY/MD
 Sample : P1062-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH266

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rVB	35329	37706	11.48%	1.306%
2	1.535	146	154	170	rBV	37738	47923	14.59%	1.659%
3	2.063	308	318	335	rVB	65061	97558	29.71%	3.378%
4	2.519	447	460	471	rBV3	17383	31138	9.48%	1.078%
5	3.812	851	862	907	rBV2	28785	110758	33.73%	3.835%
6	4.252	984	999	1029	rBV2	54346	141424	43.07%	4.897%
7	4.960	1204	1219	1245	rBV2	125001	317797	96.78%	11.005%
8	5.535	1388	1398	1427	rBV	127175	268805	81.86%	9.308%
9	5.992	1527	1540	1570	rBV	73798	159418	48.55%	5.520%
10	6.921	1819	1829	1857	rBV	33123	67355	20.51%	2.332%
11	7.246	1919	1930	1952	rBV	149531	270647	82.42%	9.372%
12	7.561	2018	2028	2052	rBV	18153	35709	10.87%	1.237%
13	7.876	2116	2126	2136	rBV3	2680	4890	1.49%	0.169%
14	8.030	2165	2174	2217	rBV	139820	315197	95.99%	10.915%
15	8.786	2399	2409	2434	rBV	195357	328381	100.00%	11.371%
16	10.156	2824	2835	2857	rBV	45974	74593	22.72%	2.583%
17	10.326	2879	2888	2899	rBV4	6466	10152	3.09%	0.352%
18	11.185	3145	3155	3180	rBV	203663	328346	99.99%	11.370%
19	11.561	3262	3272	3288	rBV	151160	240067	73.11%	8.313%




Sum of corrected areas: 2887864

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033667.D
Acq On : 16 Jan 2024 13:48
Operator : SY/MD
Sample : P1062-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

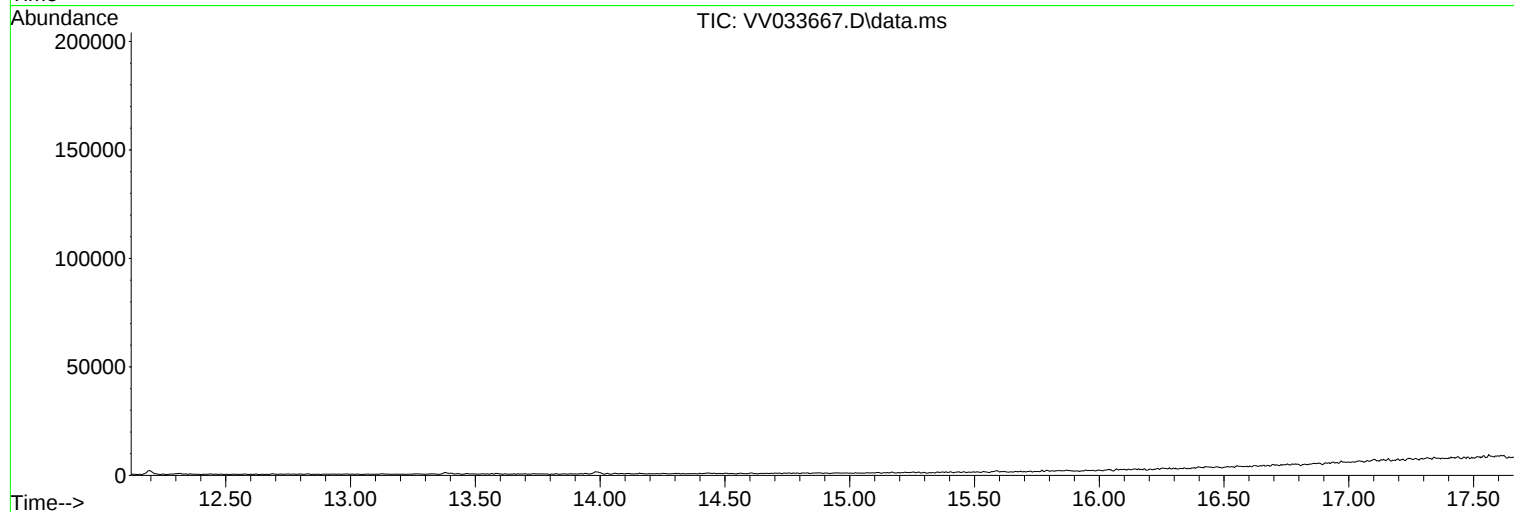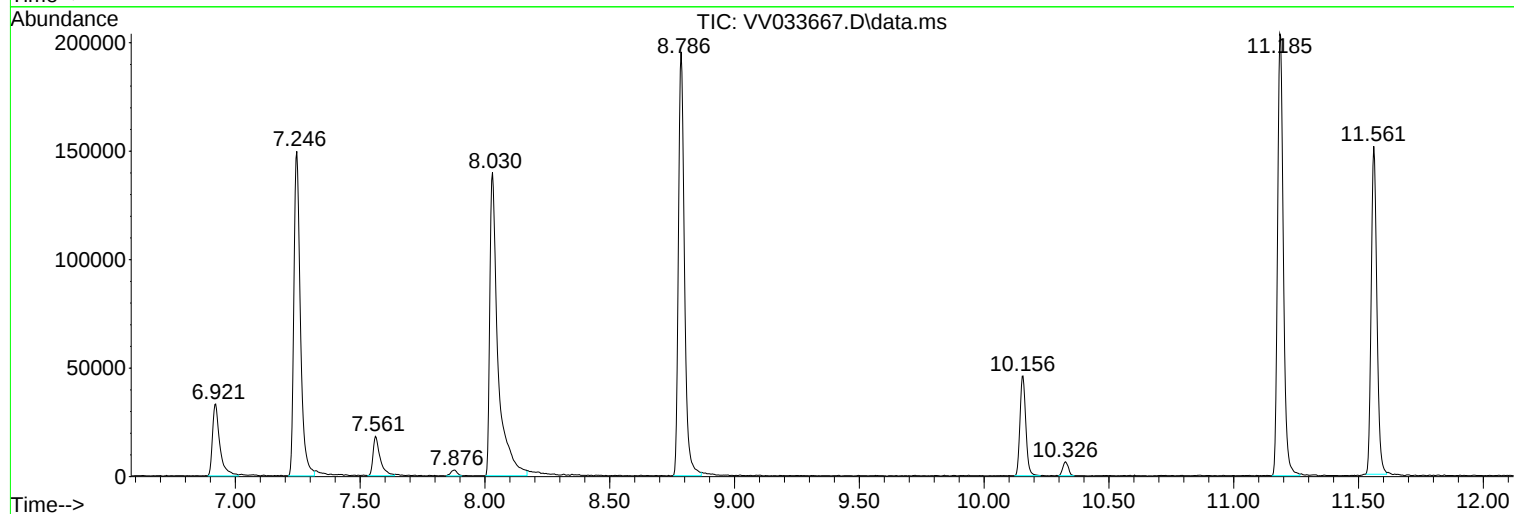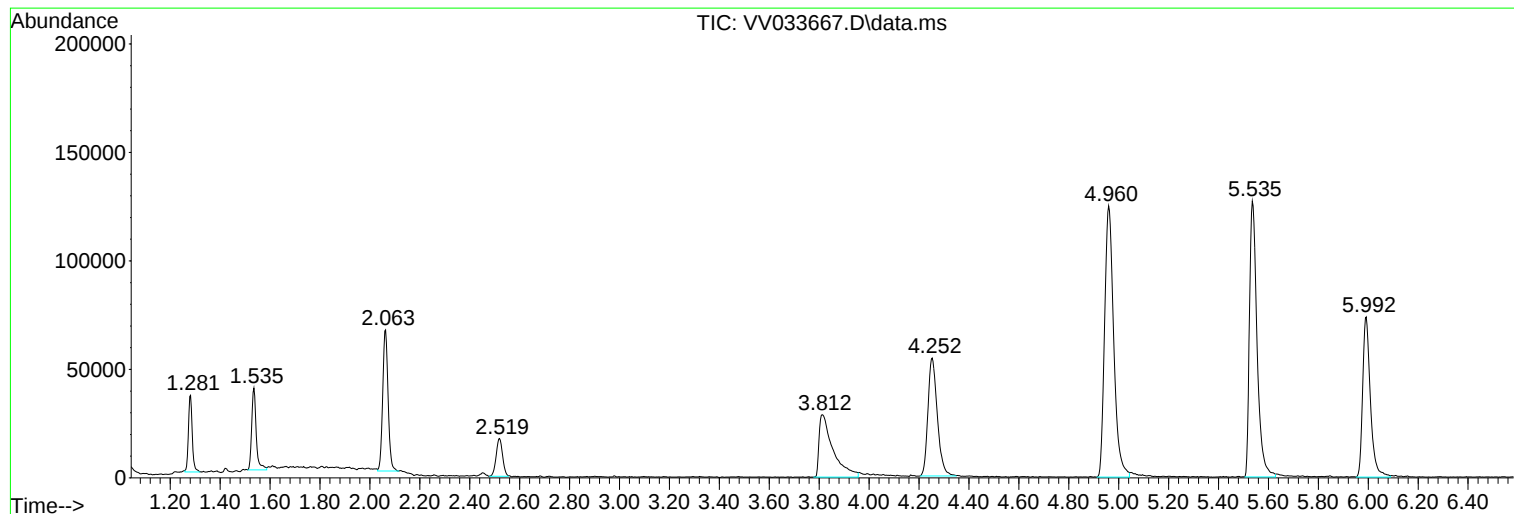

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033667.D
Acq On : 16 Jan 2024 13:48
Operator : SY/MD
Sample : P1062-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH266










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic2.519 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.519	0.58 ug/L	31138	1,4-Difluorobenzene	5.535

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentane	70	C5H10	000287-92-3	86
2			Cyclobutane, methyl-	70	C5H10	000598-61-8	86
3			Cyclopentane	70	C5H10	000287-92-3	78
4			Cyclopentane	70	C5H10	000287-92-3	78
5			Cyclobutane, methyl-	70	C5H10	000598-61-8	72

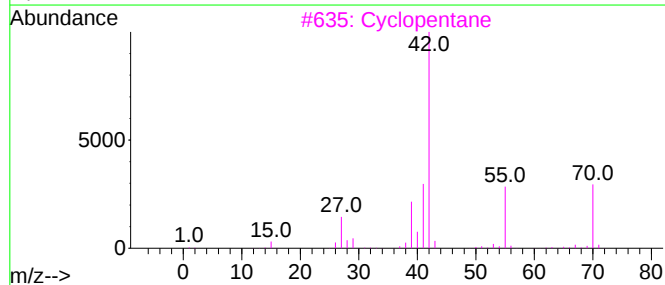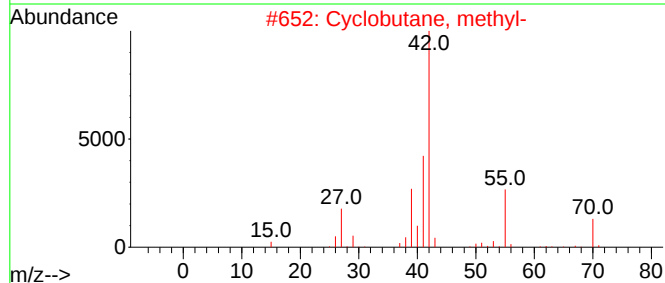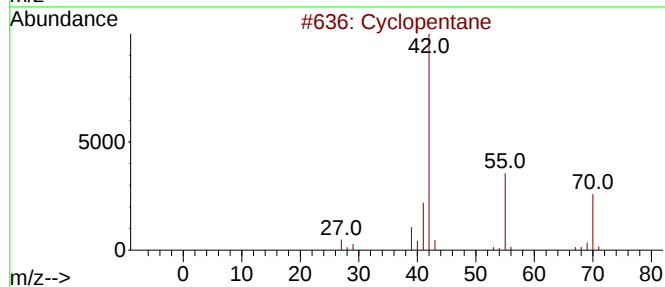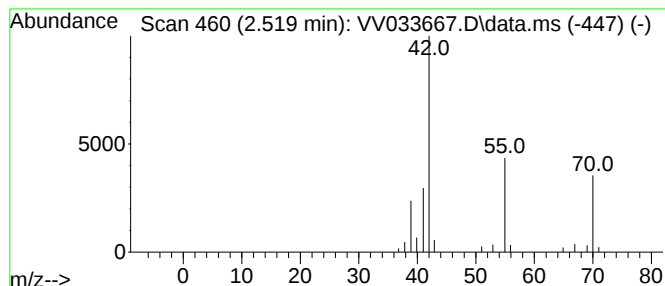

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033667.D
Acq On : 16 Jan 2024 13:48
Operator : SY/MD
Sample : P1062-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	2.519	0.6	ug/L	31138	1	5.535	268805	5.0