

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033670.D
 Acq On : 16 Jan 2024 14:59
 Operator : SY/MD
 Sample : P1062-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH269

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	35018	38190	11.53%	1.289%
2	1.536	146	154	167	rVB	37623	44832	13.54%	1.514%
3	2.063	308	318	330	rVB	66808	98092	29.63%	3.312%
4	2.519	448	460	474	rBV	29623	53404	16.13%	1.803%
5	3.825	855	866	905	rBV2	26738	111156	33.57%	3.753%
6	4.252	982	999	1024	rBV2	55711	147625	44.59%	4.984%
7	4.960	1205	1219	1248	rBV2	127375	325927	98.44%	11.005%
8	5.535	1388	1398	1423	rBV	128728	268392	81.07%	9.062%
9	5.992	1527	1540	1563	rBV2	74213	159503	48.18%	5.385%
10	6.921	1818	1829	1856	rBV2	33314	68583	20.71%	2.316%
11	7.246	1916	1930	1952	rBV	148847	273561	82.63%	9.236%
12	7.561	2018	2028	2050	rBV2	17912	36626	11.06%	1.237%
13	7.876	2115	2126	2135	rBV2	2937	4784	1.44%	0.162%
14	8.030	2165	2174	2227	rBV	141011	328559	99.24%	11.093%
15	8.786	2398	2409	2441	rBV	191492	331082	100.00%	11.179%
16	10.153	2824	2834	2855	rBV	48624	78952	23.85%	2.666%
17	10.326	2877	2888	2900	rVB2	7643	12297	3.71%	0.415%
18	11.185	3145	3155	3183	rBV	207398	329339	99.47%	11.120%
19	11.561	3262	3272	3295	rVB	157886	250835	75.76%	8.469%




Sum of corrected areas: 2961739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033670.D
Acq On : 16 Jan 2024 14:59
Operator : SY/MD
Sample : P1062-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

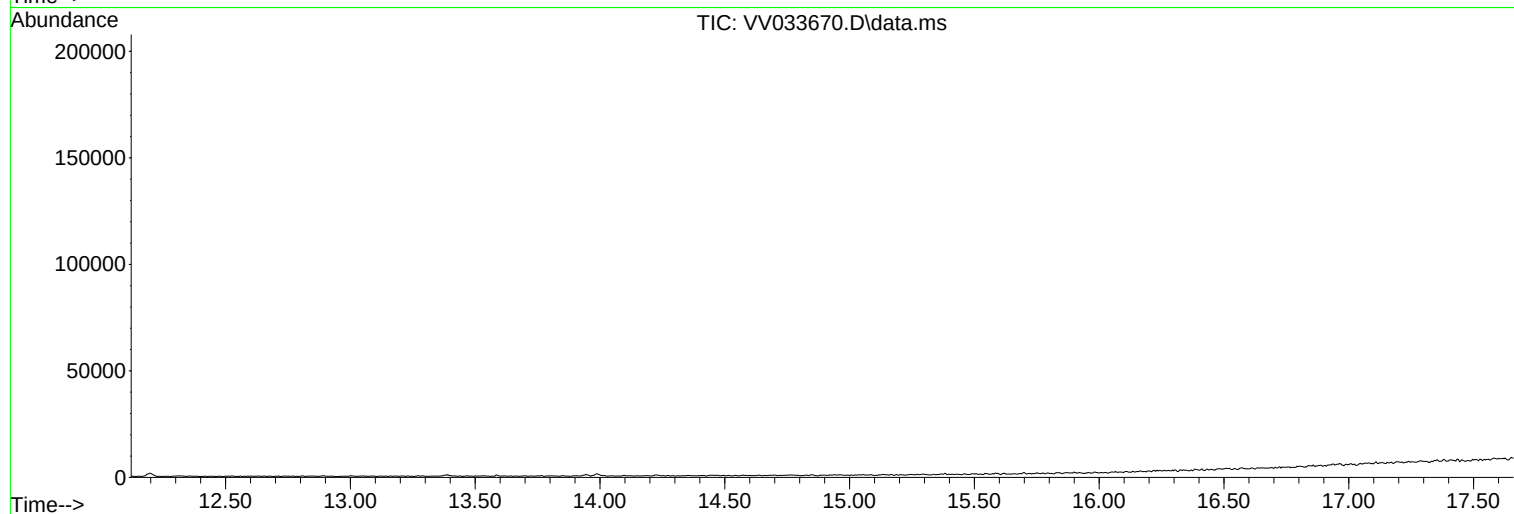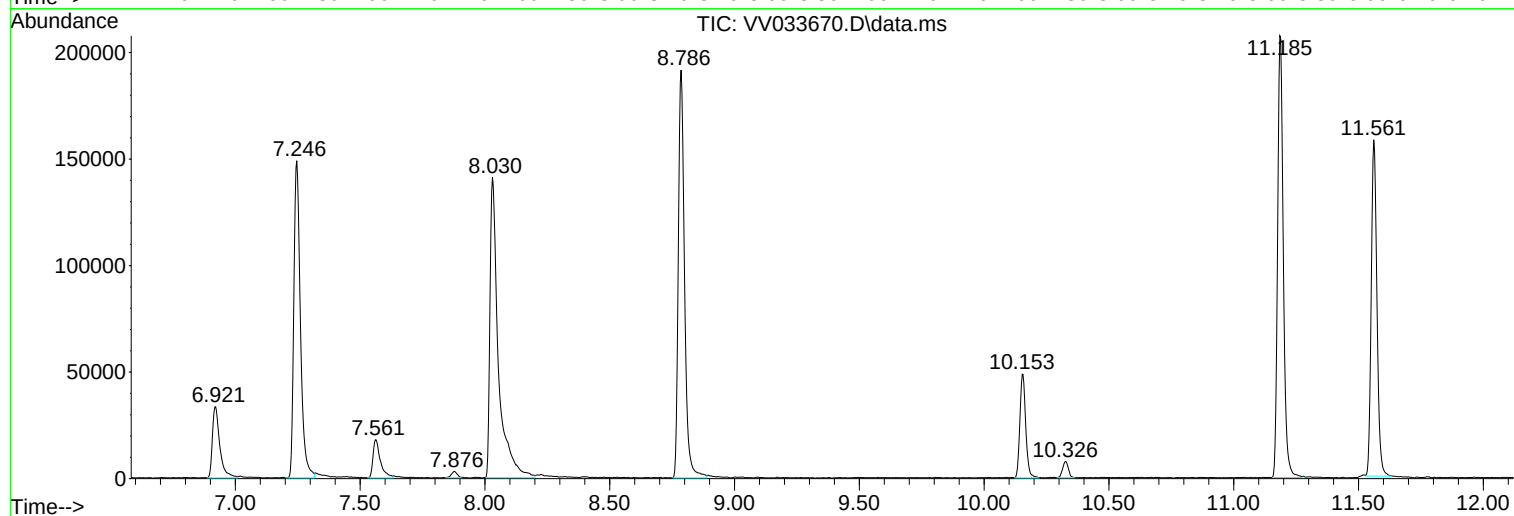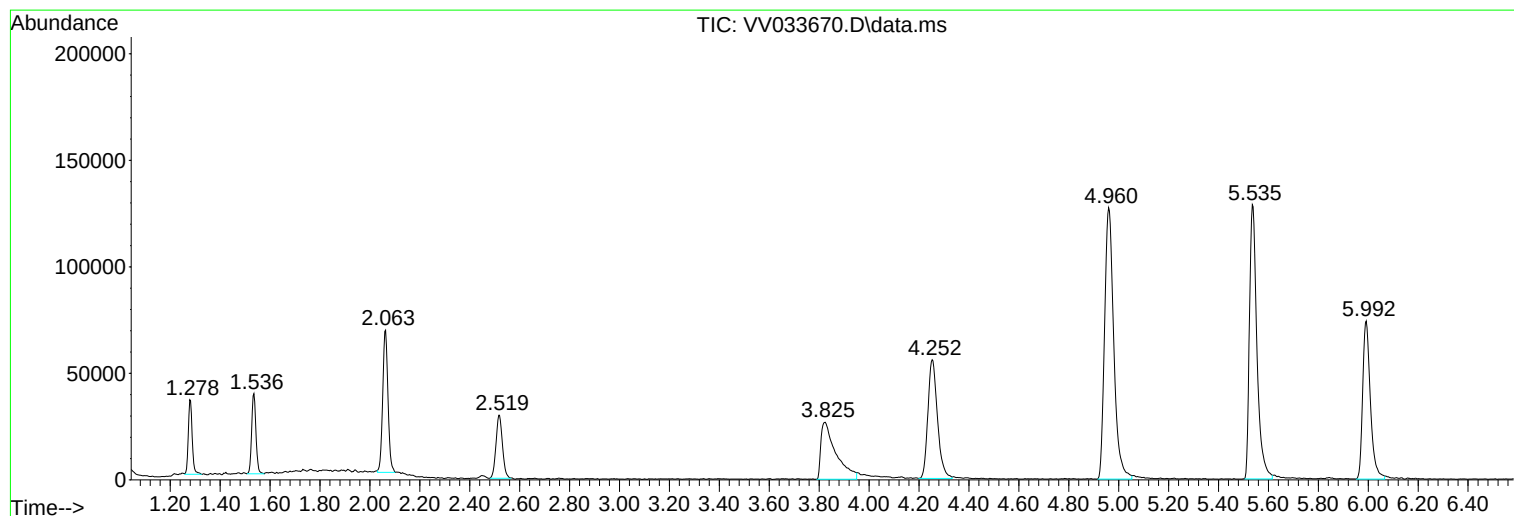

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033670.D
Acq On : 16 Jan 2024 14:59
Operator : SY/MD
Sample : P1062-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH269










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.519	0.99 ug/L	53404	1,4-Difluorobenzene	5.539

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Pentene	70	C5H10	000109-67-1	90
2		Cyclopentane	70	C5H10	000287-92-3	90
3		Cyclobutane, methyl-	70	C5H10	000598-61-8	86
4		Cyclopentane	70	C5H10	000287-92-3	78
5		Cyclopentane	70	C5H10	000287-92-3	72

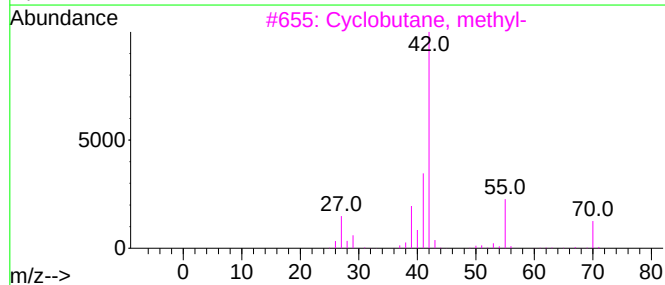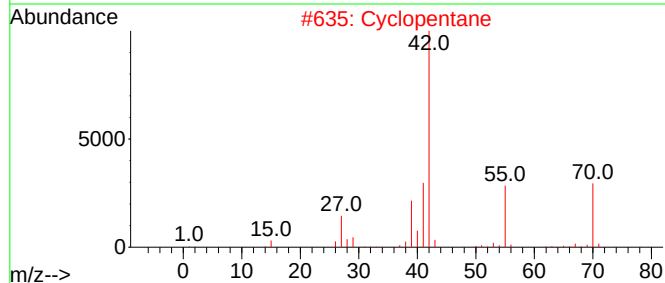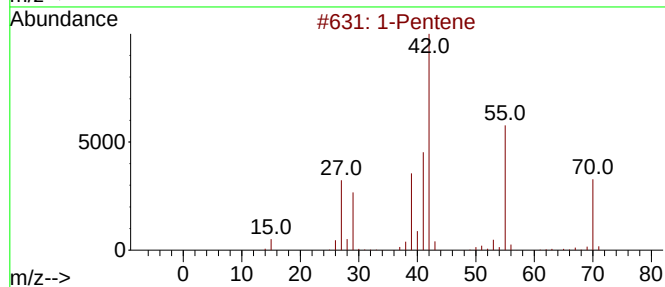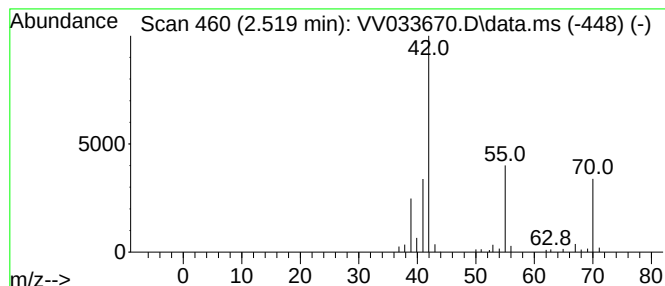

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033670.D
Acq On : 16 Jan 2024 14:59
Operator : SY/MD
Sample : P1062-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	2.519	1.0	ug/L	53404	1	5.539	268392	5.0