

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033672.D
 Acq On : 16 Jan 2024 15:47
 Operator : SY/MD
 Sample : P1062-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH271

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV033672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	27	rVB4	3712	4643	1.41%	0.144%
2	1.282	67	75	86	rVB2	46308	50369	15.25%	1.566%
3	1.536	146	154	168	rBV	35438	43219	13.08%	1.344%
4	1.767	222	226	233	rVB2	4461	4763	1.44%	0.148%
5	2.063	308	318	331	rVV	65029	100151	30.32%	3.114%
6	2.159	333	348	363	rVB3	18346	39064	11.83%	1.215%
7	2.706	508	518	533	rBV2	7643	15635	4.73%	0.486%
8	3.114	632	645	668	rVB	14547	31240	9.46%	0.971%
9	3.812	851	862	888	rBV2	40637	132752	40.19%	4.128%
10	4.253	985	999	1026	rBV	53393	140512	42.54%	4.369%
11	4.960	1205	1219	1254	rBV2	119943	307906	93.21%	9.573%
12	5.535	1383	1398	1428	rBV	126677	267966	81.12%	8.332%
13	5.835	1479	1491	1526	rBV	100863	207411	62.79%	6.449%
14	5.992	1526	1540	1569	rVV	69739	150963	45.70%	4.694%
15	6.921	1819	1829	1855	rBV2	30597	63834	19.32%	1.985%
16	7.246	1918	1930	1946	rBV	140854	253787	76.83%	7.891%
17	7.323	1946	1954	1970	rVB2	24074	46741	14.15%	1.453%
18	7.561	2020	2028	2050	rBV	17156	34318	10.39%	1.067%
19	7.912	2128	2137	2152	rVB3	13039	23648	7.16%	0.735%
20	8.031	2165	2174	2215	rBV	139854	313638	94.95%	9.752%
21	8.786	2397	2409	2440	rBV	191321	325144	98.43%	10.109%
22	9.085	2492	2502	2514	rBV2	4228	6943	2.10%	0.216%
23	10.153	2823	2834	2848	rBV	47969	76849	23.26%	2.389%
24	10.326	2879	2888	2897	rBV4	4265	6831	2.07%	0.212%
25	11.185	3145	3155	3182	rBV	205750	330332	100.00%	10.271%
26	11.561	3262	3272	3291	rVB	147495	237607	71.93%	7.388%




Sum of corrected areas: 3216266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033672.D
Acq On : 16 Jan 2024 15:47
Operator : SY/MD
Sample : P1062-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

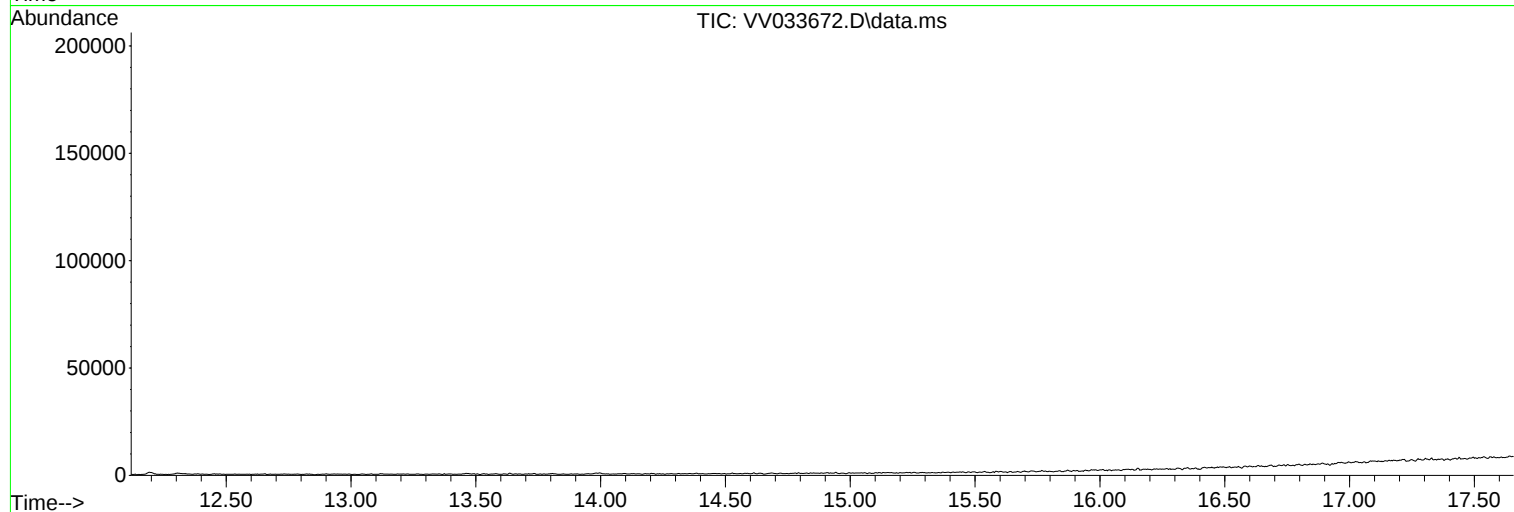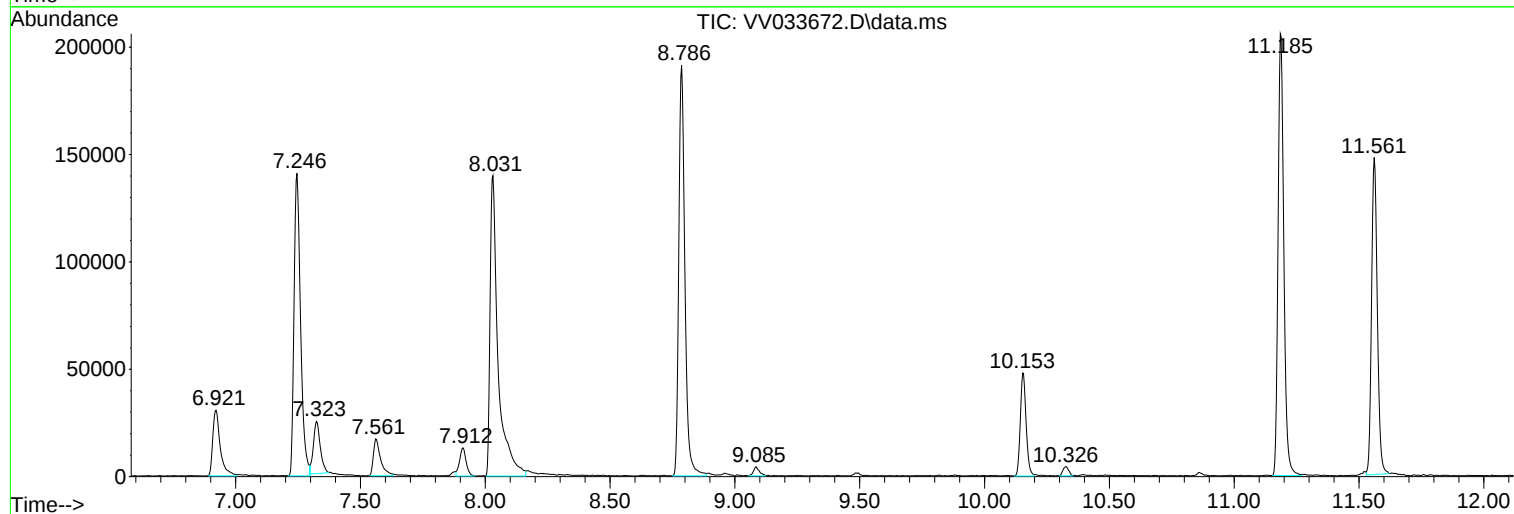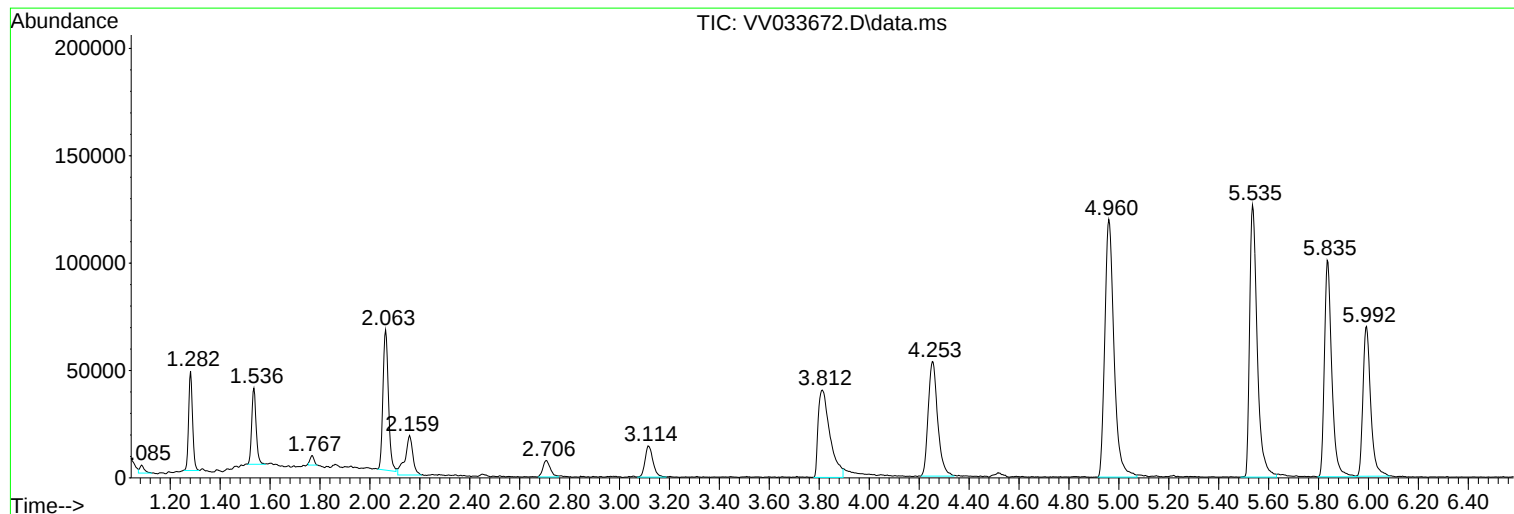

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033672.D
Acq On : 16 Jan 2024 15:47
Operator : SY/MD
Sample : P1062-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033672.D
Acq On : 16 Jan 2024 15:47
Operator : SY/MD
Sample : P1062-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc