

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033676.D
 Acq On : 16 Jan 2024 17:21
 Operator : SY/MD
 Sample : P1062-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWK1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	39	46	66	rBV	9053	29823	7.96%	0.978%
2	1.278	68	74	82	rBV	34434	36414	9.71%	1.194%
3	1.330	82	90	95	rBV2	7816	14056	3.75%	0.461%
4	1.536	147	154	175	rVB	38023	48109	12.84%	1.578%
5	2.063	308	318	334	rVB	67249	103501	27.61%	3.394%
6	3.806	851	860	895	rBV	32253	104035	27.76%	3.412%
7	4.252	983	999	1028	rBV	55638	146031	38.96%	4.789%
8	4.960	1205	1219	1250	rBV3	126068	321681	85.82%	10.549%
9	5.535	1384	1398	1434	rBV	148917	308508	82.31%	10.117%
10	5.992	1525	1540	1570	rBV	74040	159679	42.60%	5.237%
11	6.918	1818	1828	1859	rBV	32897	67700	18.06%	2.220%
12	7.246	1918	1930	1951	rBV	149914	270908	72.28%	8.884%
13	7.561	2019	2028	2049	rBV2	17168	34834	9.29%	1.142%
14	8.027	2164	2173	2211	rBV	144220	319029	85.11%	10.462%
15	8.786	2398	2409	2437	rBV	219872	370899	98.95%	12.163%
16	10.156	2824	2835	2863	rVB	48761	78768	21.01%	2.583%
17	10.326	2879	2888	2897	rVB3	3237	4642	1.24%	0.152%
18	11.185	3136	3155	3181	rBV	237758	374825	100.00%	12.292%
19	11.519	3248	3259	3262	rBV5	2475	4470	1.19%	0.147%
20	11.561	3262	3272	3298	rVB	153569	251431	67.08%	8.245%




Sum of corrected areas: 3049343

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033676.D
Acq On : 16 Jan 2024 17:21
Operator : SY/MD
Sample : P1062-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

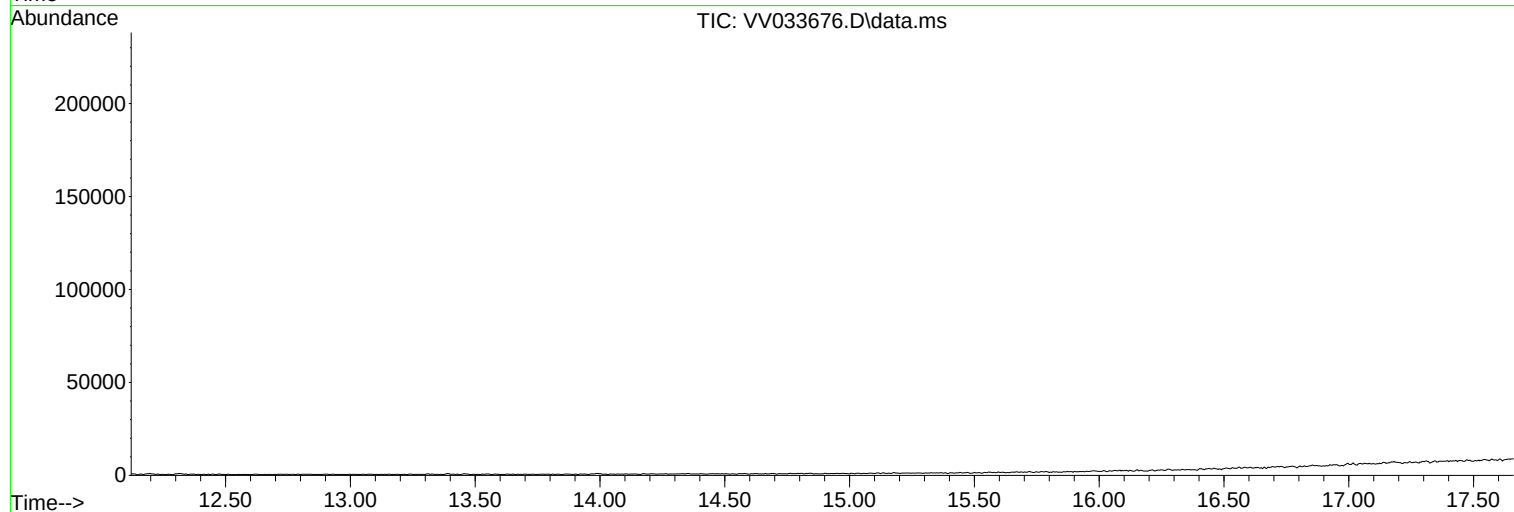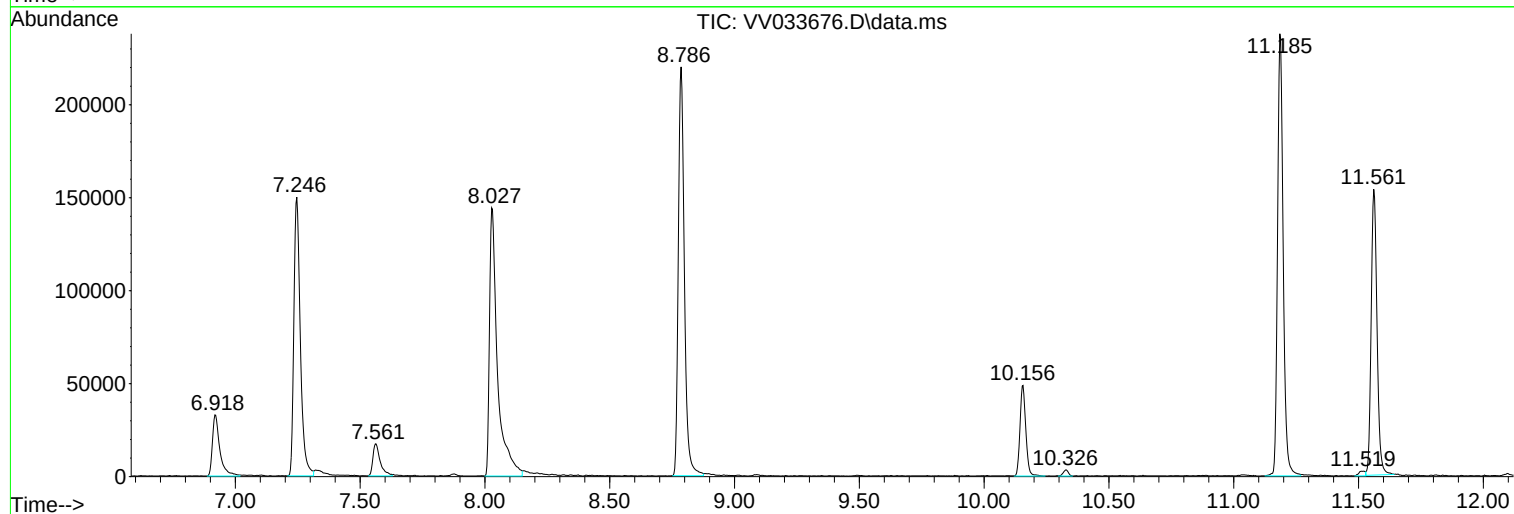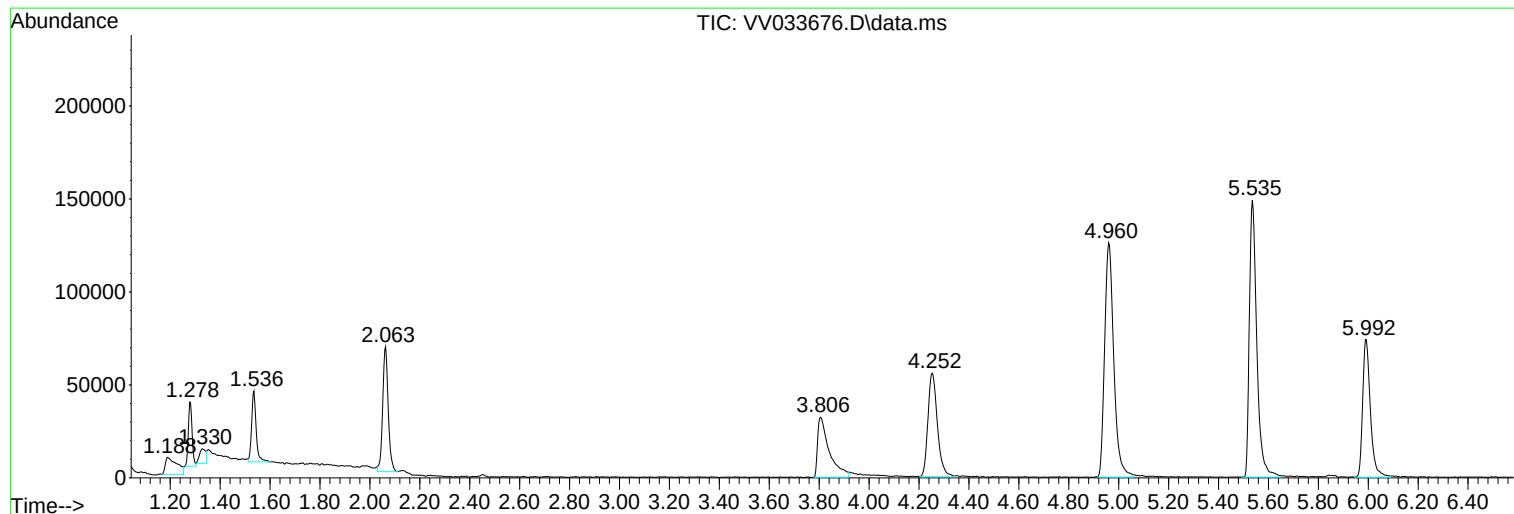

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033676.D
Acq On : 16 Jan 2024 17:21
Operator : SY/MD
Sample : P1062-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033676.D
Acq On : 16 Jan 2024 17:21
Operator : SY/MD
Sample : P1062-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc