

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033681.D
 Acq On : 16 Jan 2024 19:20
 Operator : SY/MD
 Sample : P1131-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV033681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.223	40	57	62	rBV4	4503	11126	3.45%	0.400%
2	1.278	65	74	87	rVB2	35003	47111	14.61%	1.695%
3	1.535	147	154	165	rVB	34157	40180	12.46%	1.446%
4	2.063	309	318	334	rVV	60991	93102	28.87%	3.350%
5	2.127	335	338	352	rVB5	2581	4513	1.40%	0.162%
6	3.812	853	862	903	rBV	29487	109813	34.05%	3.952%
7	4.256	984	1000	1032	rBV2	53305	158481	49.14%	5.703%
8	4.960	1204	1219	1254	rBV3	115806	300041	93.04%	10.797%
9	5.535	1388	1398	1432	rBV	116485	250428	77.66%	9.012%
10	5.992	1524	1540	1566	rBV	68668	148433	46.03%	5.341%
11	6.918	1817	1828	1849	rBV	31938	64203	19.91%	2.310%
12	7.246	1917	1930	1948	rBV	134844	245638	76.17%	8.839%
13	7.329	1950	1956	1968	rVB3	4785	9393	2.91%	0.338%
14	7.561	2019	2028	2050	rBV2	16494	33980	10.54%	1.223%
15	8.030	2165	2174	2220	rBV	134582	313898	97.34%	11.296%
16	8.786	2399	2409	2437	rBV	182844	307316	95.30%	11.059%
17	10.156	2818	2835	2857	rBV	46223	74450	23.09%	2.679%
18	10.323	2879	2887	2898	rBV3	2681	4540	1.41%	0.163%
19	11.184	3145	3155	3180	rBV	196504	322481	100.00%	11.604%
20	11.561	3257	3272	3293	rBV	144748	239832	74.37%	8.630%




Sum of corrected areas: 2778959

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033681.D
Acq On : 16 Jan 2024 19:20
Operator : SY/MD
Sample : P1131-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

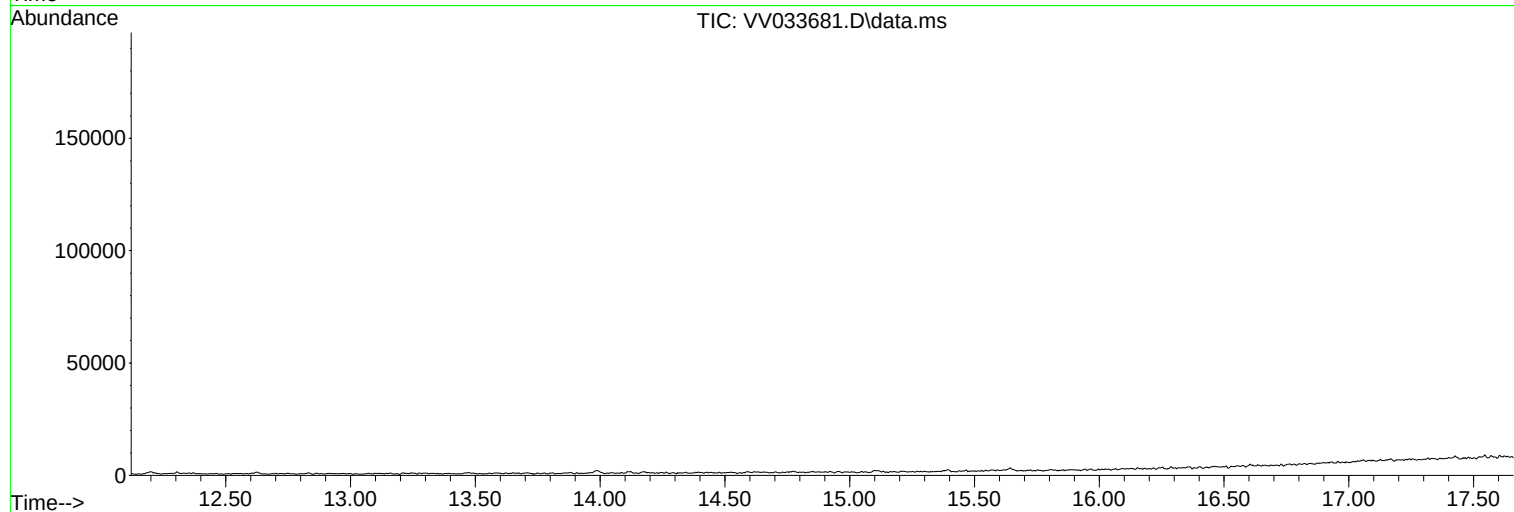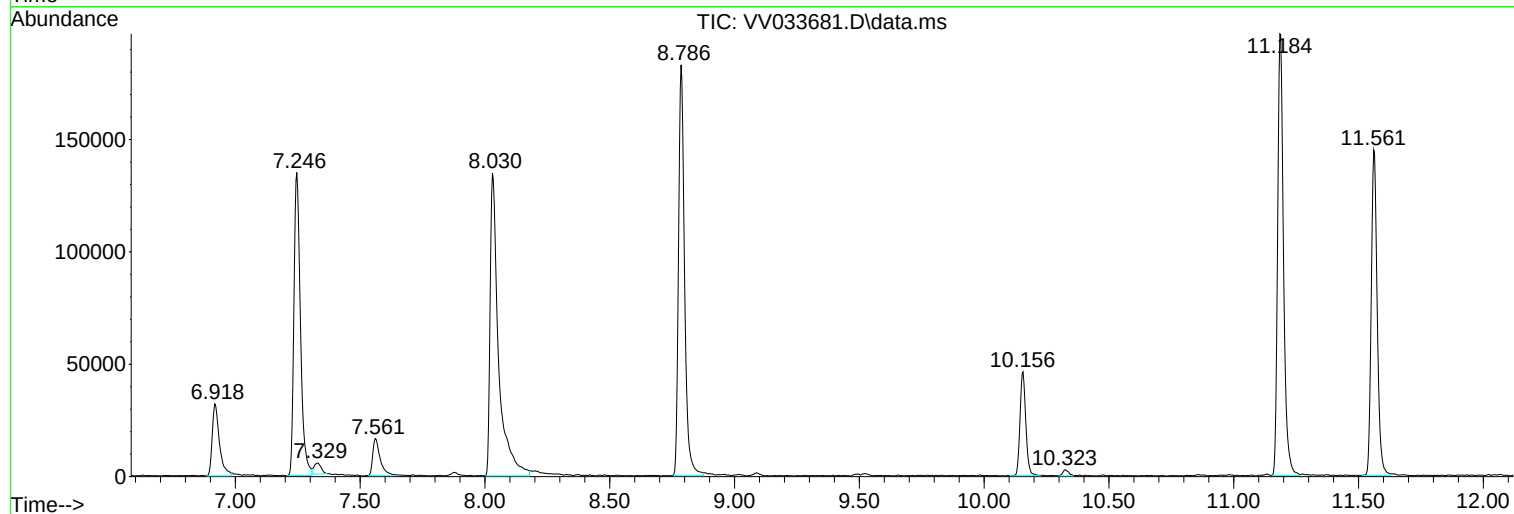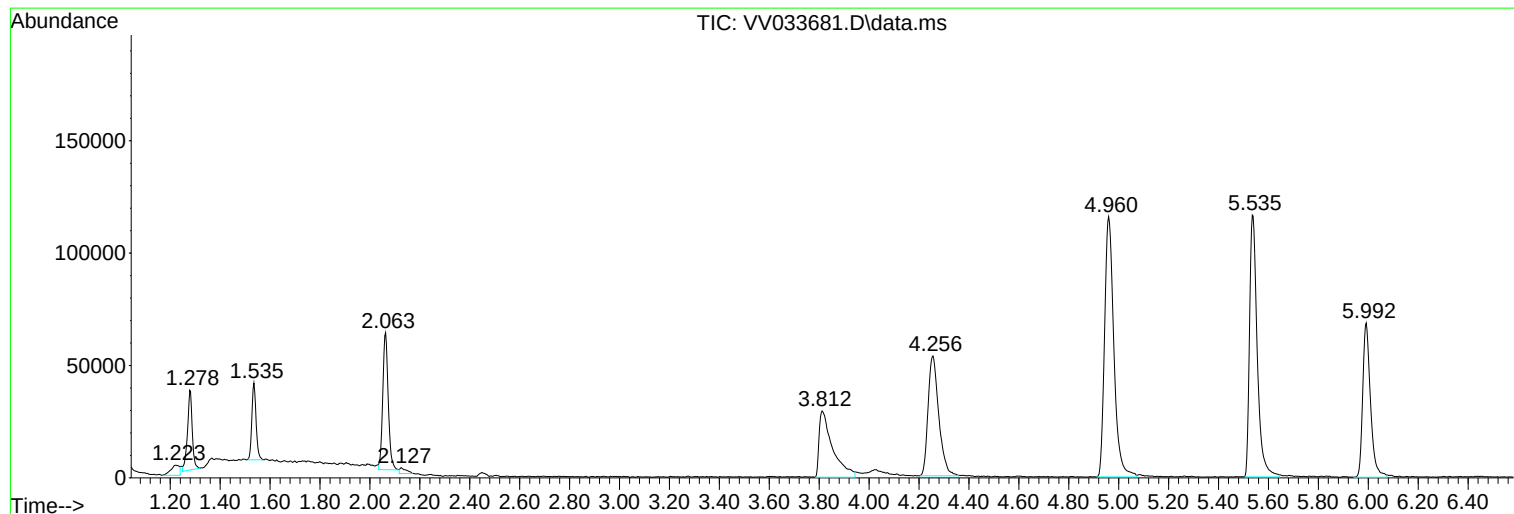

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033681.D
Acq On : 16 Jan 2024 19:20
Operator : SY/MD
Sample : P1131-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033681.D
Acq On : 16 Jan 2024 19:20
Operator : SY/MD
Sample : P1131-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
