

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033683.D
 Acq On : 16 Jan 2024 20:31
 Operator : SY/MD
 Sample : VV0116WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK396

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	82	rBV	36564	38097	11.66%	1.352%
2	1.535	147	154	165	rVB	37262	43763	13.39%	1.553%
3	2.060	308	317	342	rVB	67602	106750	32.66%	3.788%
4	2.445	432	437	448	rVB5	2306	3971	1.22%	0.141%
5	3.822	855	865	896	rBV	27483	107205	32.80%	3.804%
6	4.252	982	999	1029	rBV2	55240	144965	44.36%	5.144%
7	4.960	1200	1219	1252	rBV2	124895	317920	97.28%	11.280%
8	5.535	1388	1398	1430	rBV	123718	262088	80.19%	9.299%
9	5.992	1527	1540	1578	rBV	73063	159382	48.77%	5.655%
10	6.918	1819	1828	1849	rBV	33038	66981	20.49%	2.377%
11	7.246	1919	1930	1954	rBV	146211	265429	81.21%	9.418%
12	7.561	2018	2028	2045	rBV	18601	35955	11.00%	1.276%
13	8.030	2165	2174	2225	rBV	140881	326824	100.00%	11.596%
14	8.786	2399	2409	2437	rBV	185725	318029	97.31%	11.284%
15	10.156	2824	2835	2860	rBV	49147	80101	24.51%	2.842%
16	10.329	2880	2889	2900	rVB	2217	3390	1.04%	0.120%
17	11.188	3145	3156	3177	rBV	185220	299138	91.53%	10.614%
18	11.561	3262	3272	3296	rBV	140162	229788	70.31%	8.153%
19	13.455	3850	3861	3871	rBV	2863	4408	1.35%	0.156%
20	13.988	4015	4027	4036	rBV2	2523	4221	1.29%	0.150%




Sum of corrected areas: 2818405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033683.D
Acq On : 16 Jan 2024 20:31
Operator : SY/MD
Sample : VV0116WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK396

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

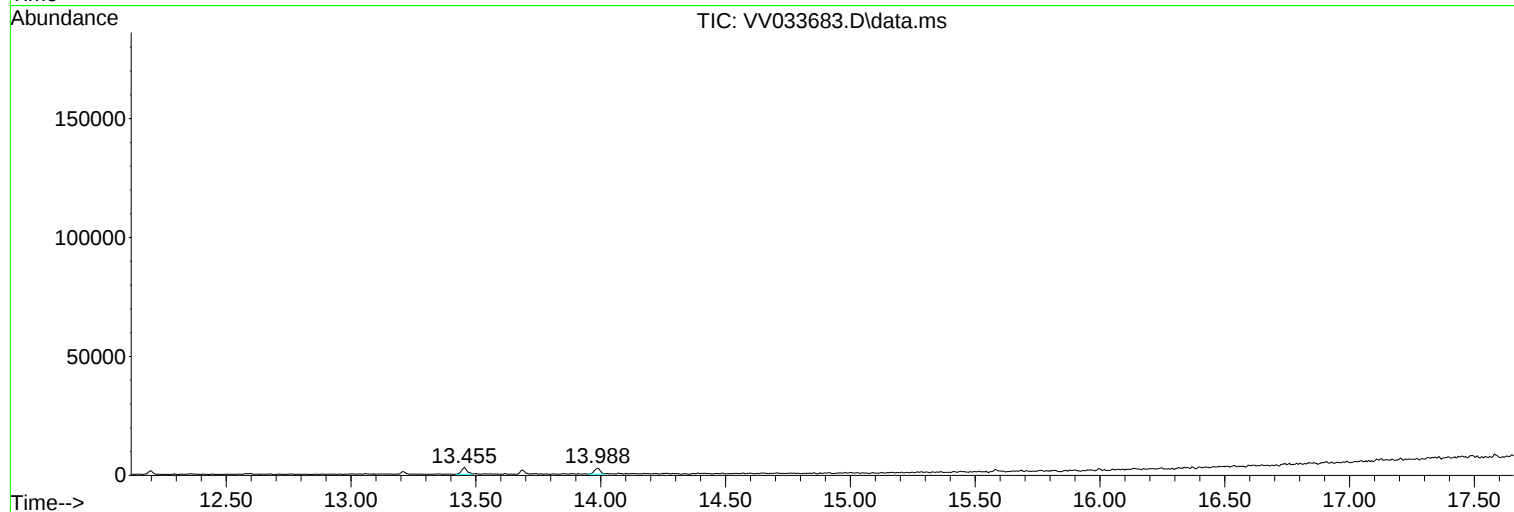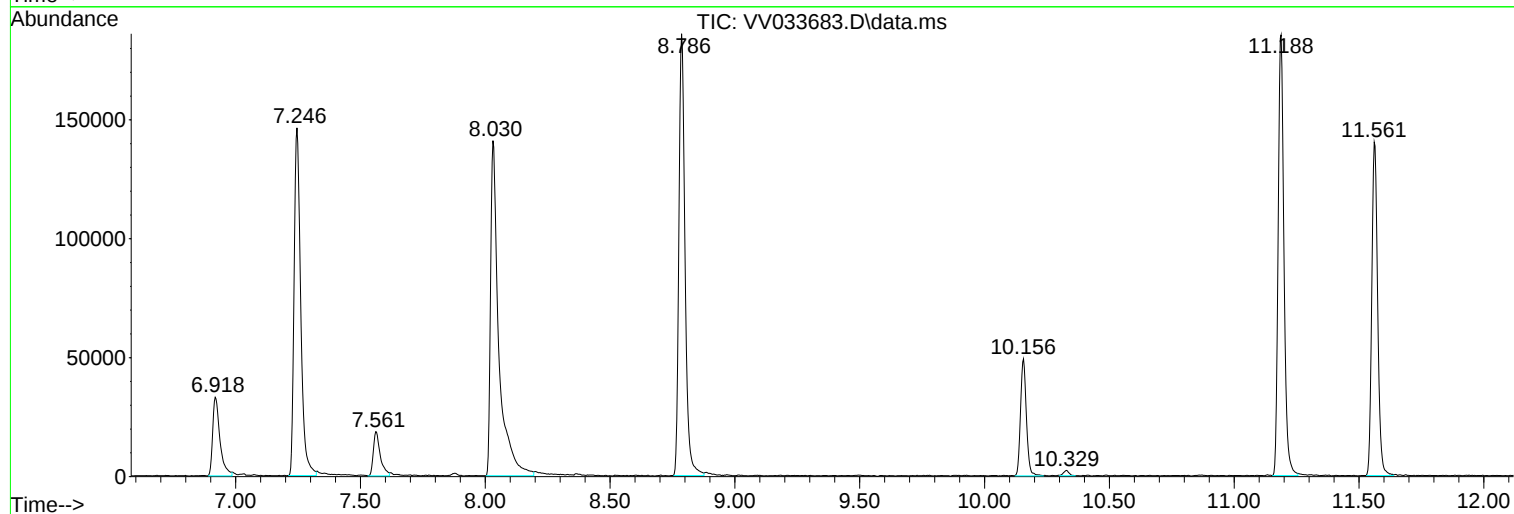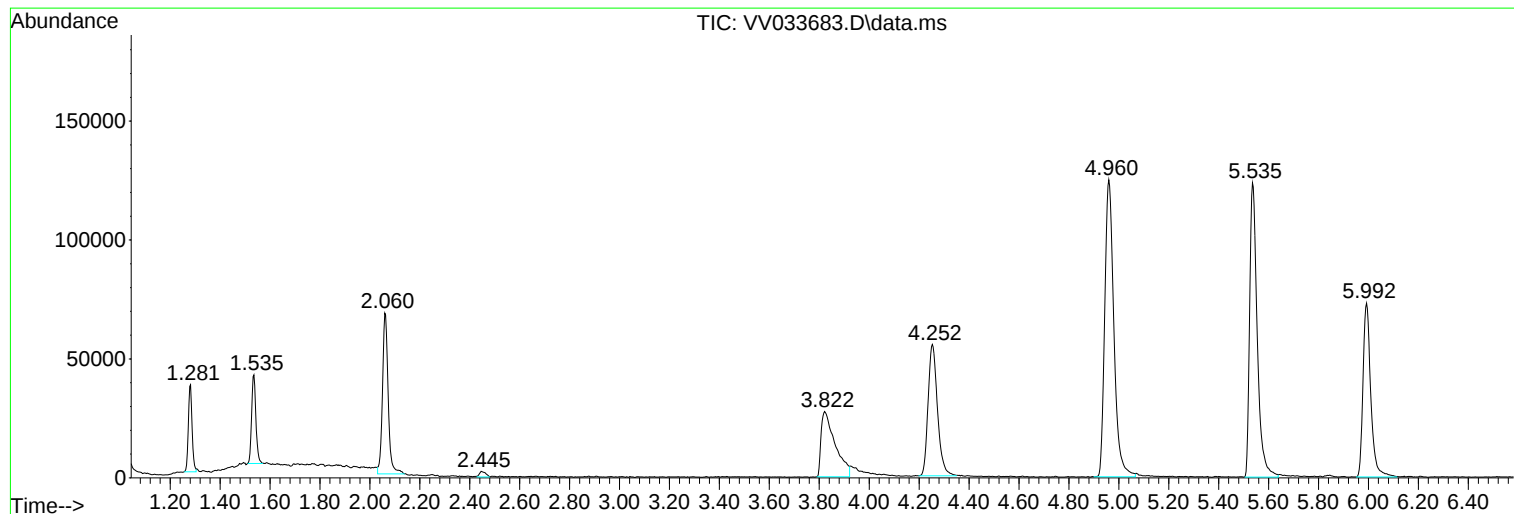

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033683.D
Acq On : 16 Jan 2024 20:31
Operator : SY/MD
Sample : VV0116WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK396

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033683.D
Acq On : 16 Jan 2024 20:31
Operator : SY/MD
Sample : VV0116WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK396

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc