

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033688.D
 Acq On : 16 Jan 2024 22:34
 Operator : SY/MD
 Sample : P1120-14DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWJ0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	86	rVB2	35773	39012	11.68%	1.258%
2	1.535	147	154	165	rBV	34340	40011	11.98%	1.290%
3	2.063	308	318	336	rVB	64575	99762	29.87%	3.217%
4	2.452	430	439	450	rVB2	5069	8699	2.60%	0.281%
5	3.812	849	862	898	rBV4	45687	156235	46.78%	5.038%
6	4.252	984	999	1025	rBV	53929	140217	41.99%	4.521%
7	4.960	1205	1219	1255	rBV2	120929	310949	93.11%	10.027%
8	5.535	1388	1398	1425	rBV	126369	266601	79.83%	8.597%
9	5.834	1480	1491	1522	rBV	100094	210168	62.93%	6.777%
10	5.992	1528	1540	1571	rBV	70915	150666	45.11%	4.858%
11	6.918	1819	1828	1851	rBV3	34096	67496	20.21%	2.176%
12	7.246	1918	1930	1954	rBV	140725	257618	77.14%	8.307%
13	7.561	2020	2028	2046	rBV2	18306	35286	10.57%	1.138%
14	8.030	2164	2174	2219	rBV	148081	329697	98.72%	10.631%
15	8.786	2399	2409	2432	rBV	195945	325911	97.59%	10.509%
16	10.156	2824	2835	2853	rBV	49148	78334	23.46%	2.526%
17	10.326	2880	2888	2898	rVB2	2572	3949	1.18%	0.127%
18	11.185	3145	3155	3179	rBV	206671	333963	100.00%	10.769%
19	11.561	3261	3272	3297	rBV	149481	246615	73.85%	7.952%




Sum of corrected areas: 3101189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033688.D
Acq On : 16 Jan 2024 22:34
Operator : SY/MD
Sample : P1120-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWJ0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

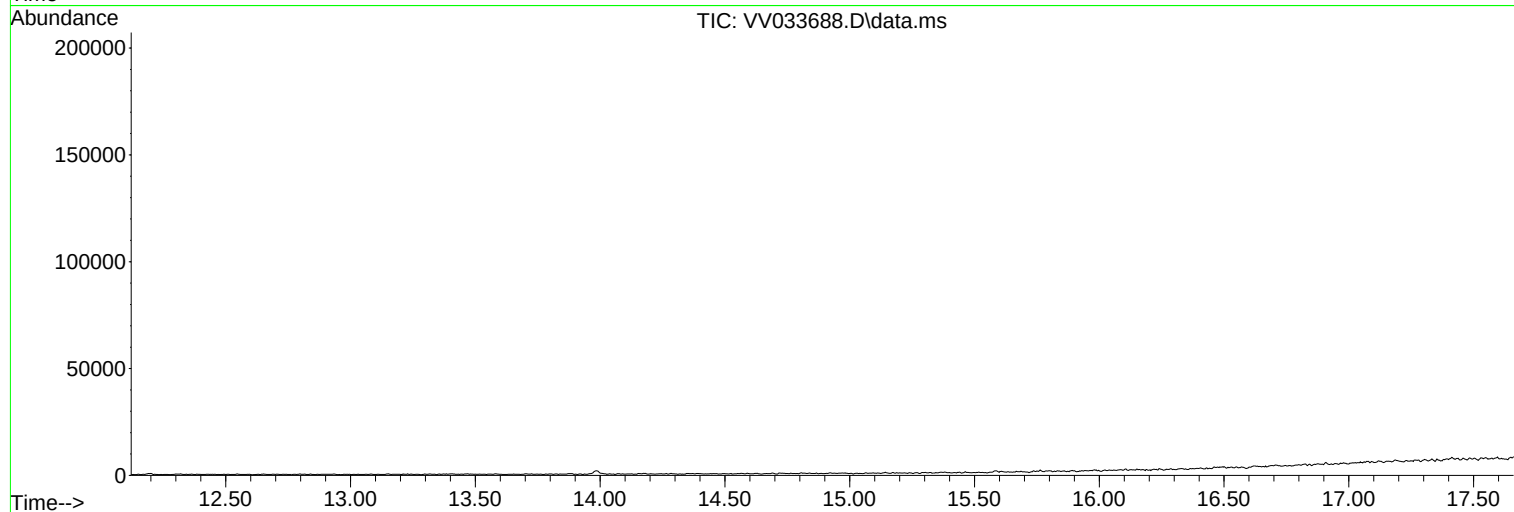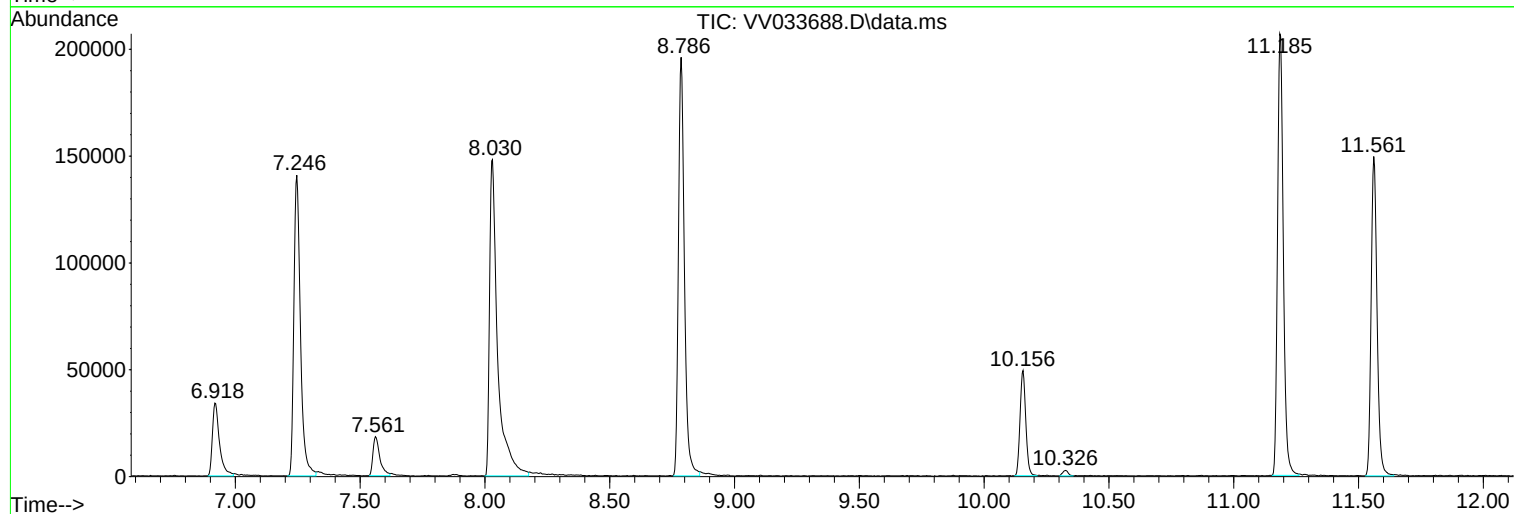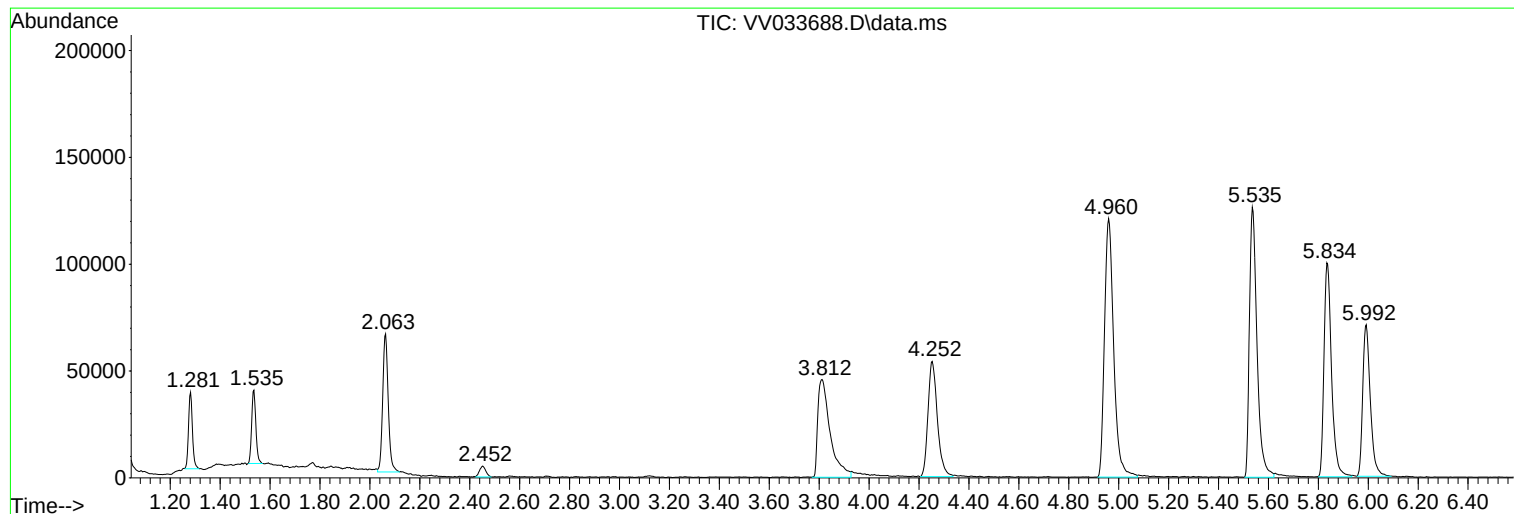

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033688.D
Acq On : 16 Jan 2024 22:34
Operator : SY/MD
Sample : P1120-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWJ0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033688.D
Acq On : 16 Jan 2024 22:34
Operator : SY/MD
Sample : P1120-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWJ0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc