

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033690.D
 Acq On : 16 Jan 2024 23:21
 Operator : SY/MD
 Sample : P1120-11DL 8X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWH7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB2	48685	55849	16.63%	1.672%
2	1.532	146	153	165	rVV	33583	42897	12.77%	1.284%
3	2.069	307	320	334	rBV4	144242	240871	71.73%	7.212%
4	2.452	429	439	452	rVB	7694	12517	3.73%	0.375%
5	2.699	506	516	537	rVB	19488	36032	10.73%	1.079%
6	3.114	630	645	670	rBV	57592	121516	36.19%	3.638%
7	3.809	848	861	893	rBV3	43656	147436	43.91%	4.414%
8	4.252	982	999	1022	rBV	50500	132138	39.35%	3.956%
9	4.960	1205	1219	1244	rBV2	112854	289395	86.18%	8.665%
10	5.535	1388	1398	1424	rBV	130157	269525	80.26%	8.070%
11	5.834	1479	1491	1522	rBV	117712	241757	71.99%	7.238%
12	5.992	1528	1540	1560	rBV	67537	141740	42.21%	4.244%
13	6.918	1819	1828	1856	rBV2	31849	63855	19.02%	1.912%
14	7.246	1918	1930	1953	rBV	133712	241259	71.85%	7.223%
15	7.561	2019	2028	2050	rBV	17570	34362	10.23%	1.029%
16	8.027	2164	2173	2220	rBV	134419	295268	87.93%	8.840%
17	8.786	2398	2409	2439	rBV	194034	328208	97.74%	9.827%
18	10.156	2823	2835	2850	rBV2	44624	73364	21.85%	2.197%
19	10.329	2878	2889	2900	rVB3	2355	4042	1.20%	0.121%
20	11.185	3145	3155	3186	rBV	210642	335801	100.00%	10.054%
21	11.561	3261	3272	3296	rBV	145094	232139	69.13%	6.950%




Sum of corrected areas: 3339971

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033690.D
Acq On : 16 Jan 2024 23:21
Operator : SY/MD
Sample : P1120-11DL 8X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWH7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

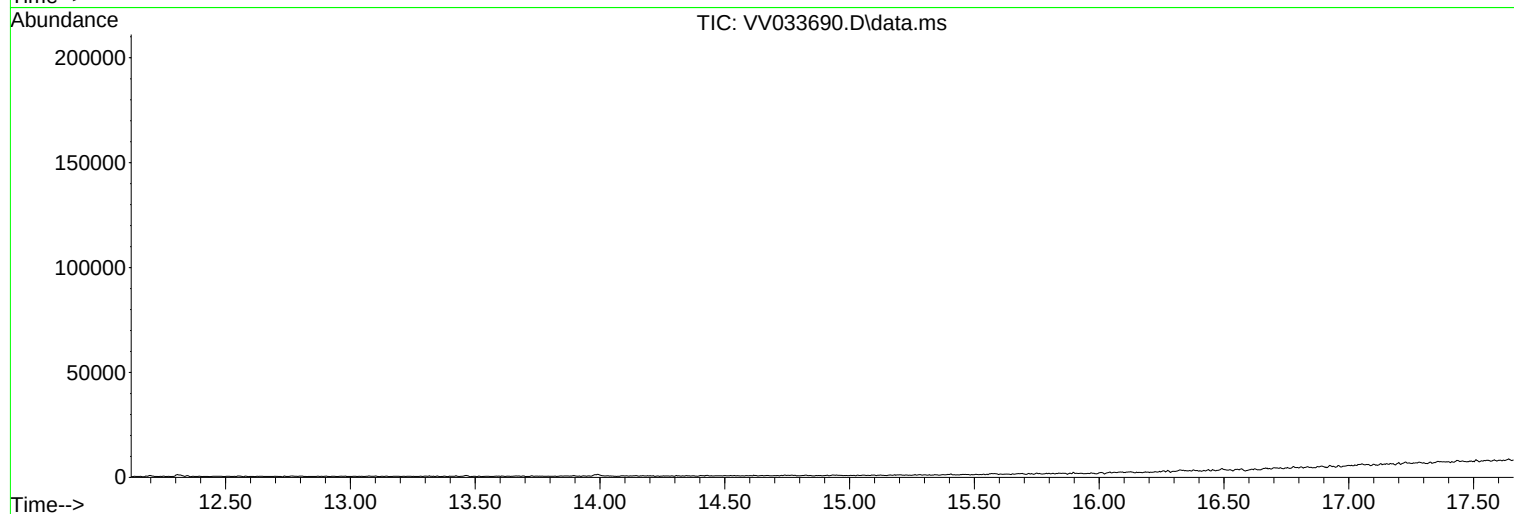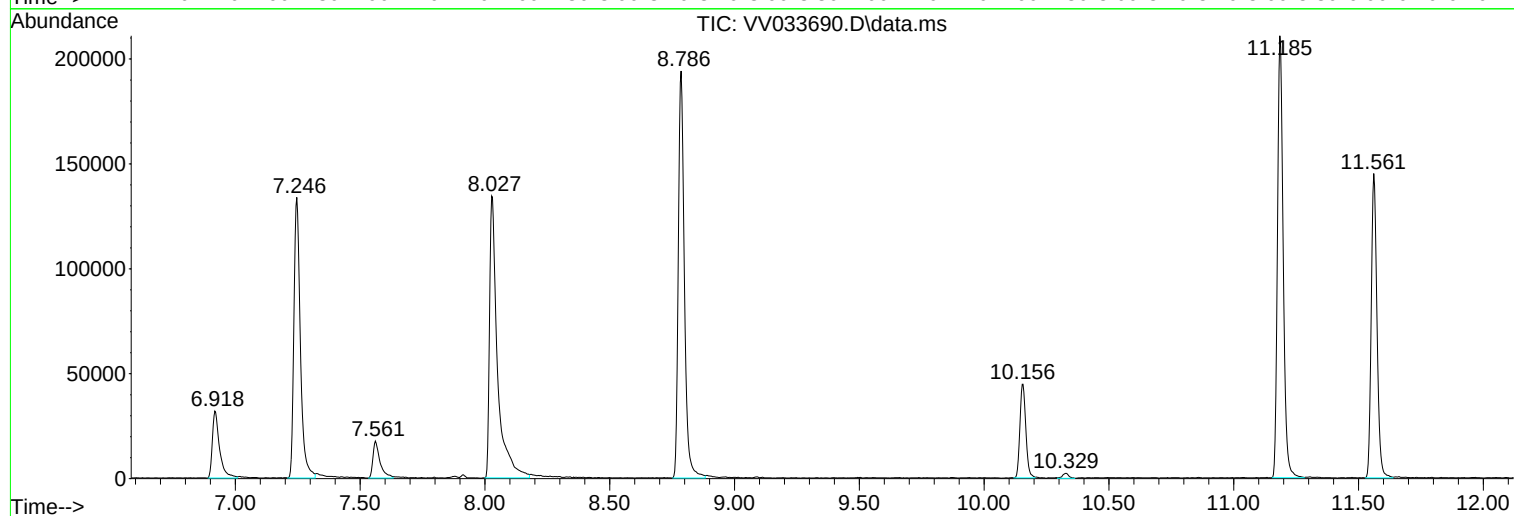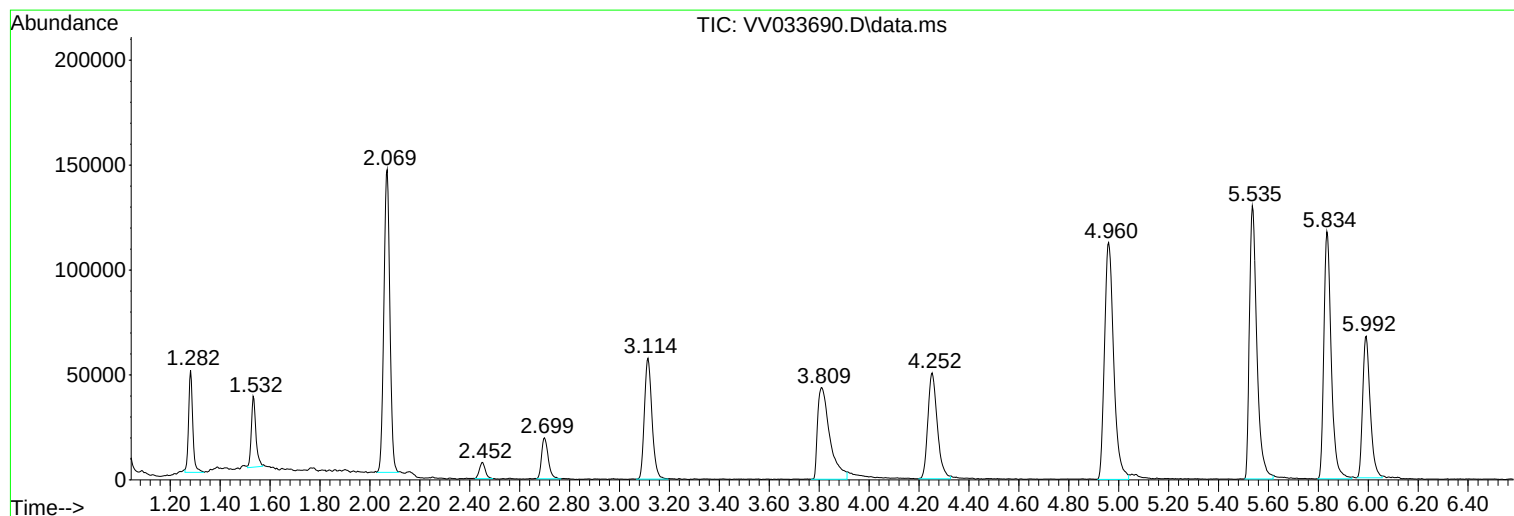

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033690.D
Acq On : 16 Jan 2024 23:21
Operator : SY/MD
Sample : P1120-11DL 8X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWH7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033690.D
Acq On : 16 Jan 2024 23:21
Operator : SY/MD
Sample : P1120-11DL 8X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWH7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc