

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033693.D
 Acq On : 17 Jan 2024 00:33
 Operator : SY/MD
 Sample : P1120-10DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWH6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rBV2	39717	43171	13.93%	1.485%
2	1.536	146	154	165	rVB	32335	38325	12.36%	1.318%
3	2.063	308	318	330	rVB2	59744	94878	30.61%	3.263%
4	2.449	428	438	450	rVB2	7345	12491	4.03%	0.430%
5	3.121	635	647	656	rBV2	3945	7585	2.45%	0.261%
6	3.815	847	863	902	rBV3	98133	291529	94.05%	10.025%
7	4.253	981	999	1024	rBV2	49371	130469	42.09%	4.487%
8	4.960	1205	1219	1250	rBV2	109270	281619	90.85%	9.685%
9	5.535	1388	1398	1428	rBV	122179	256201	82.65%	8.811%
10	5.838	1482	1492	1519	rBV3	43395	92383	29.80%	3.177%
11	5.992	1525	1540	1571	rBV2	65373	142733	46.05%	4.908%
12	6.918	1819	1828	1857	rBV	30037	61659	19.89%	2.120%
13	7.246	1919	1930	1949	rBV	121373	217214	70.08%	7.470%
14	7.561	2020	2028	2047	rBV3	16047	32371	10.44%	1.113%
15	8.031	2165	2174	2220	rBV	136814	309969	100.00%	10.660%
16	8.786	2398	2409	2439	rBV	178925	306509	98.88%	10.541%
17	10.153	2825	2834	2849	rBV	43856	71975	23.22%	2.475%
18	11.185	3145	3155	3182	rBV	190785	305165	98.45%	10.494%
19	11.561	3262	3272	3300	rBV	130720	211651	68.28%	7.278%




Sum of corrected areas: 2907897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033693.D
Acq On : 17 Jan 2024 00:33
Operator : SY/MD
Sample : P1120-10DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWH6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

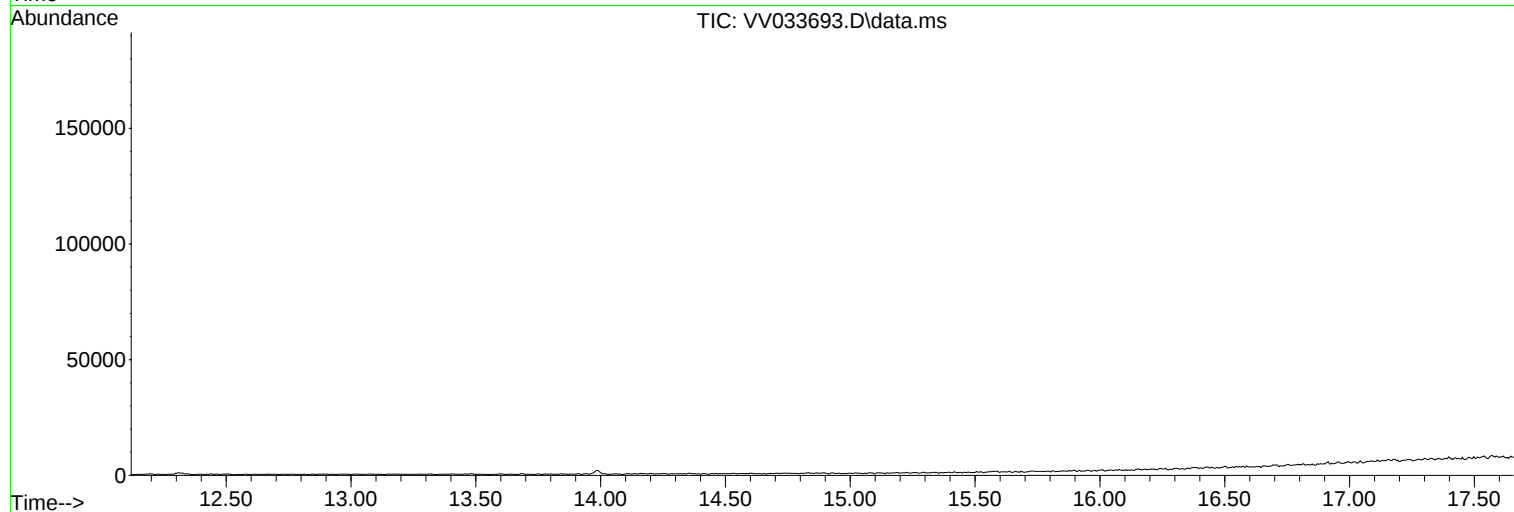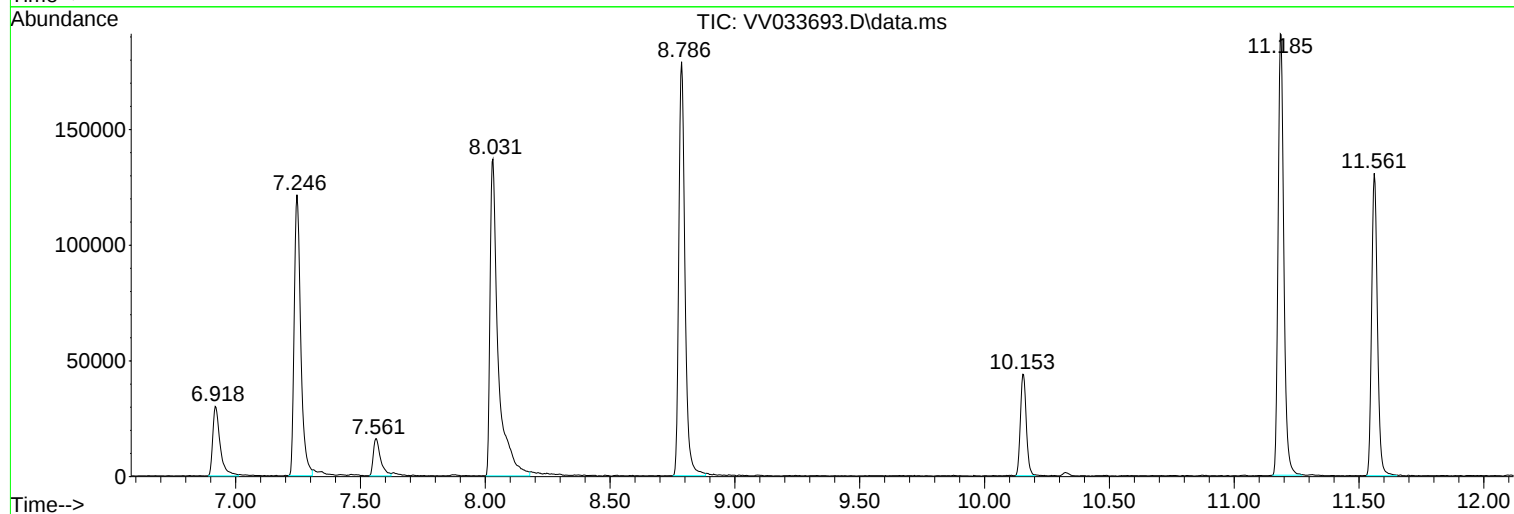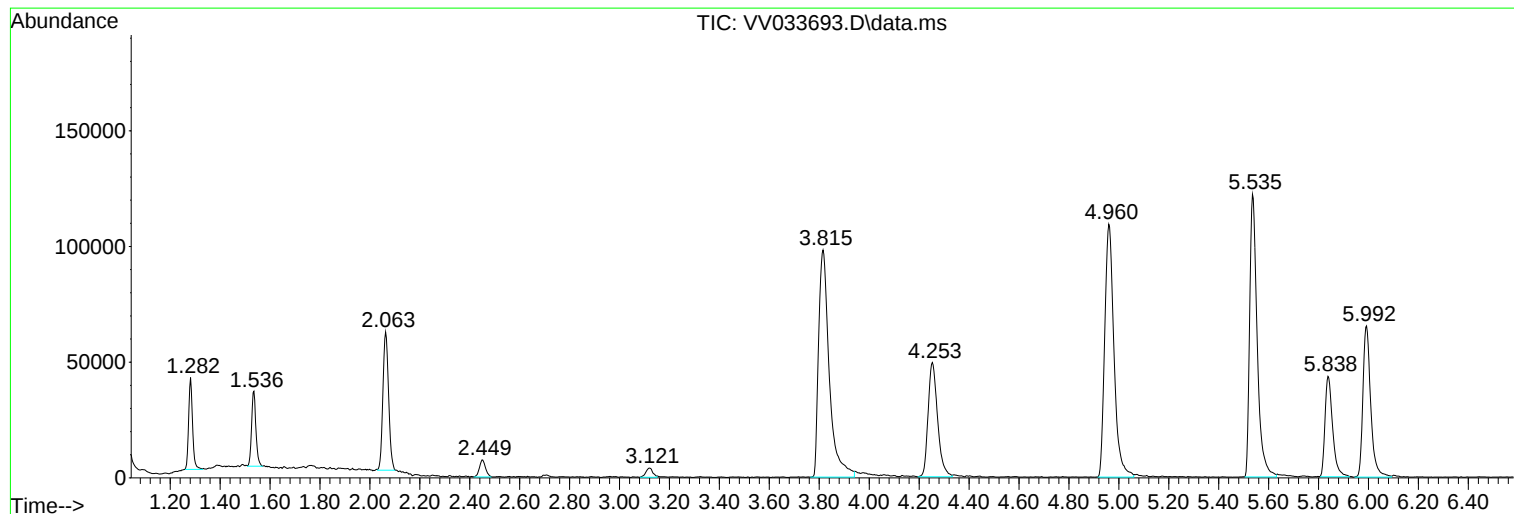

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033693.D
Acq On : 17 Jan 2024 00:33
Operator : SY/MD
Sample : P1120-10DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWH6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033693.D
Acq On : 17 Jan 2024 00:33
Operator : SY/MD
Sample : P1120-10DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWH6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc