

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033696.D
 Acq On : 17 Jan 2024 01:44
 Operator : SY/MD
 Sample : P1143-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV033696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	65	75	86	rBV	33395	39783	12.27%	1.451%
2	1.536	146	154	167	rVB	33226	38857	11.98%	1.417%
3	2.063	308	318	333	rVB	57979	86250	26.60%	3.145%
4	2.449	431	438	452	rVB4	2288	3477	1.07%	0.127%
5	3.815	854	863	890	rBV2	28149	98869	30.49%	3.605%
6	4.253	984	999	1028	rBV3	53141	155051	47.82%	5.654%
7	4.960	1204	1219	1253	rBV2	114344	293735	90.60%	10.711%
8	5.535	1387	1398	1435	rBV	124681	263357	81.23%	9.603%
9	5.992	1528	1540	1564	rBV	67906	143774	44.34%	5.243%
10	6.918	1818	1828	1858	rBV2	31294	64397	19.86%	2.348%
11	7.246	1919	1930	1950	rBV	133107	242826	74.90%	8.855%
12	7.330	1950	1956	1965	rVB4	3943	7089	2.19%	0.259%
13	7.561	2019	2028	2053	rBV2	17472	34327	10.59%	1.252%
14	8.031	2164	2174	2228	rBV	134079	307589	94.87%	11.216%
15	8.786	2398	2409	2434	rBV	188615	316899	97.74%	11.556%
16	10.153	2821	2834	2853	rBV	46723	73117	22.55%	2.666%
17	10.323	2873	2887	2900	rVB3	2866	5025	1.55%	0.183%
18	11.185	3145	3155	3178	rBV	203226	324220	100.00%	11.823%
19	11.561	3262	3272	3297	rBV	142477	230859	71.20%	8.418%
20	12.828	3658	3666	3678	rVB6	2497	3956	1.22%	0.144%
21	13.243	3791	3795	3810	rBV	8264	8883	2.74%	0.324%




Sum of corrected areas: 2742340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033696.D
Acq On : 17 Jan 2024 01:44
Operator : SY/MD
Sample : P1143-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

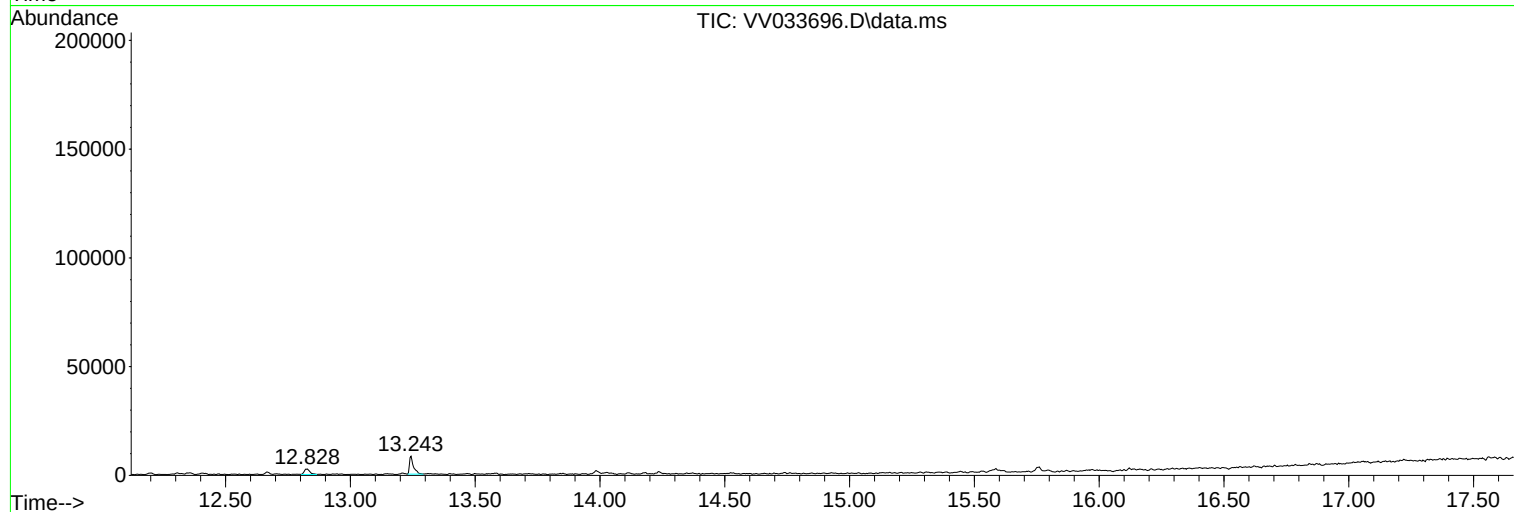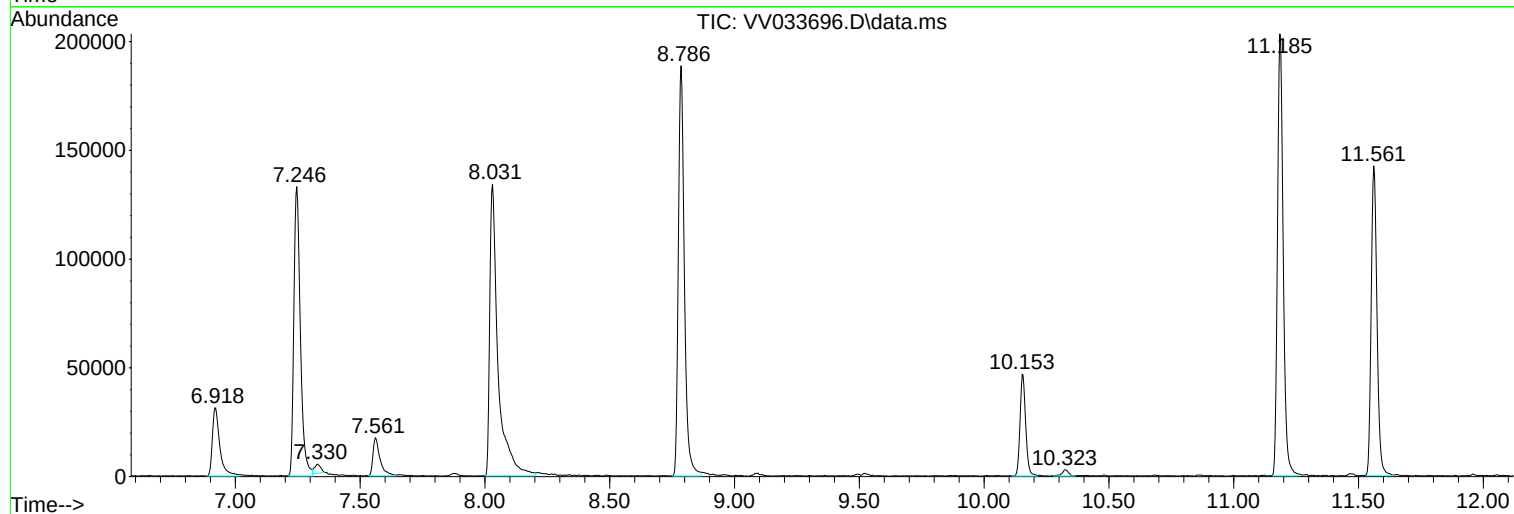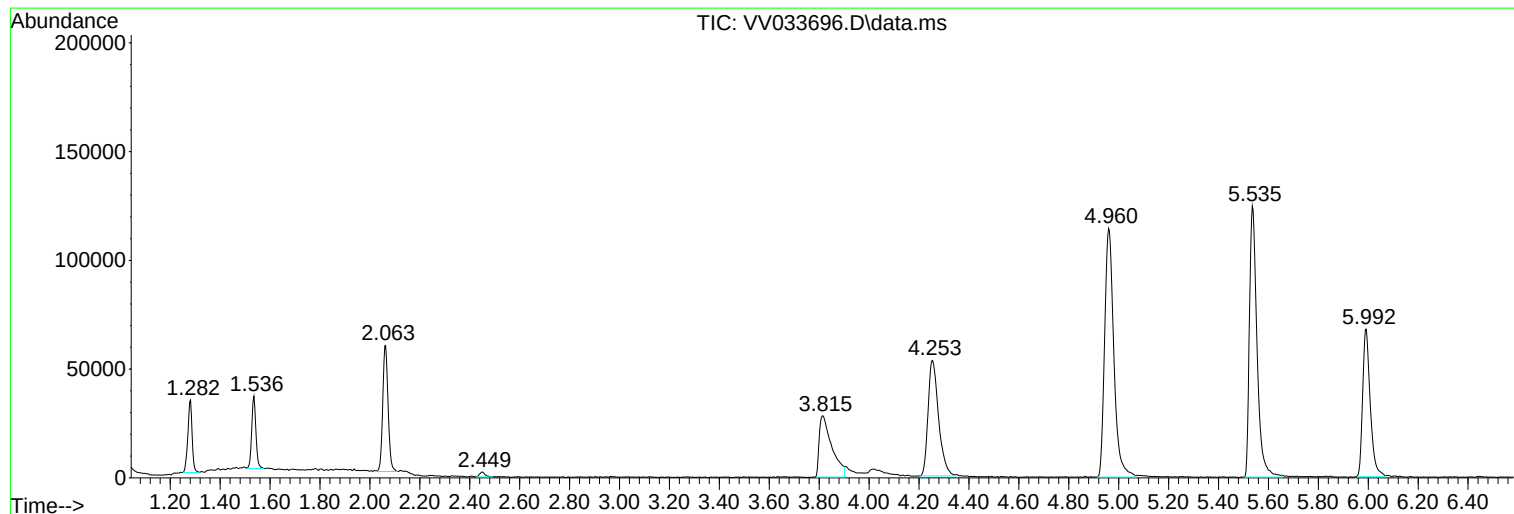

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033696.D
Acq On : 17 Jan 2024 01:44
Operator : SY/MD
Sample : P1143-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033696.D
Acq On : 17 Jan 2024 01:44
Operator : SY/MD
Sample : P1143-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc