

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
 Data File : VV033697.D
 Acq On : 17 Jan 2024 02:08
 Operator : SY/MD
 Sample : P1143-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B07

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV033697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	65	75	88	rBV	33564	41489	13.14%	1.499%
2	1.536	147	154	164	rBV	32995	39105	12.39%	1.412%
3	2.063	308	318	334	rVB	58739	88764	28.12%	3.206%
4	2.449	428	438	449	rBV5	2278	3852	1.22%	0.139%
5	3.812	851	862	895	rBV2	30108	107489	34.05%	3.882%
6	4.031	919	930	939	rBV6	1460	3526	1.12%	0.127%
7	4.256	984	1000	1029	rBV2	54602	158259	50.13%	5.716%
8	4.960	1204	1219	1255	rBV2	116676	301112	95.38%	10.876%
9	5.535	1387	1398	1435	rBV	121440	254582	80.64%	9.195%
10	5.992	1528	1540	1575	rBV2	68637	147928	46.86%	5.343%
11	6.918	1818	1828	1857	rBV	31800	66472	21.06%	2.401%
12	7.246	1917	1930	1948	rBV	138369	249994	79.19%	9.029%
13	7.330	1951	1956	1974	rVB2	5195	10445	3.31%	0.377%
14	7.561	2020	2028	2050	rBV	17821	36140	11.45%	1.305%
15	7.879	2115	2127	2136	rBV4	2225	4115	1.30%	0.149%
16	8.031	2162	2174	2218	rBV	136955	313708	99.37%	11.331%
17	8.786	2398	2409	2433	rBV	182140	307527	97.41%	11.107%
18	10.156	2824	2835	2852	rBV	46967	74175	23.50%	2.679%
19	10.326	2878	2888	2901	rVB2	5259	8393	2.66%	0.303%
20	11.185	3145	3155	3175	rBV	200183	315699	100.00%	11.403%
21	11.561	3262	3272	3299	rBV	146608	235880	74.72%	8.520%




Sum of corrected areas: 2768654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033697.D
Acq On : 17 Jan 2024 02:08
Operator : SY/MD
Sample : P1143-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

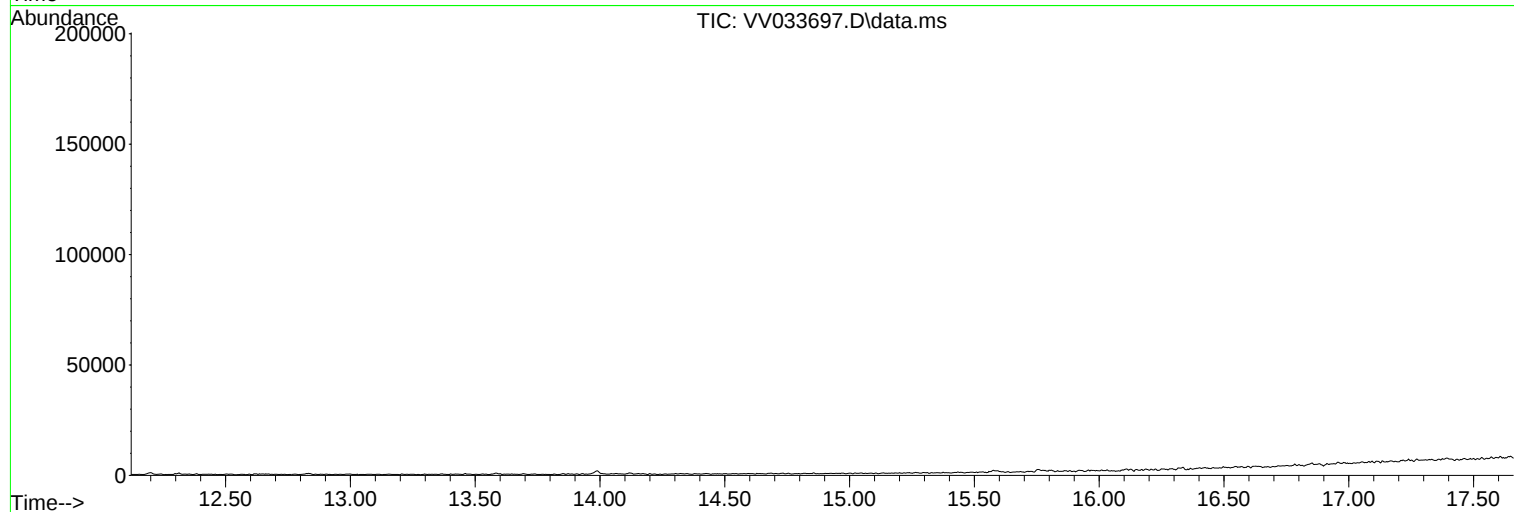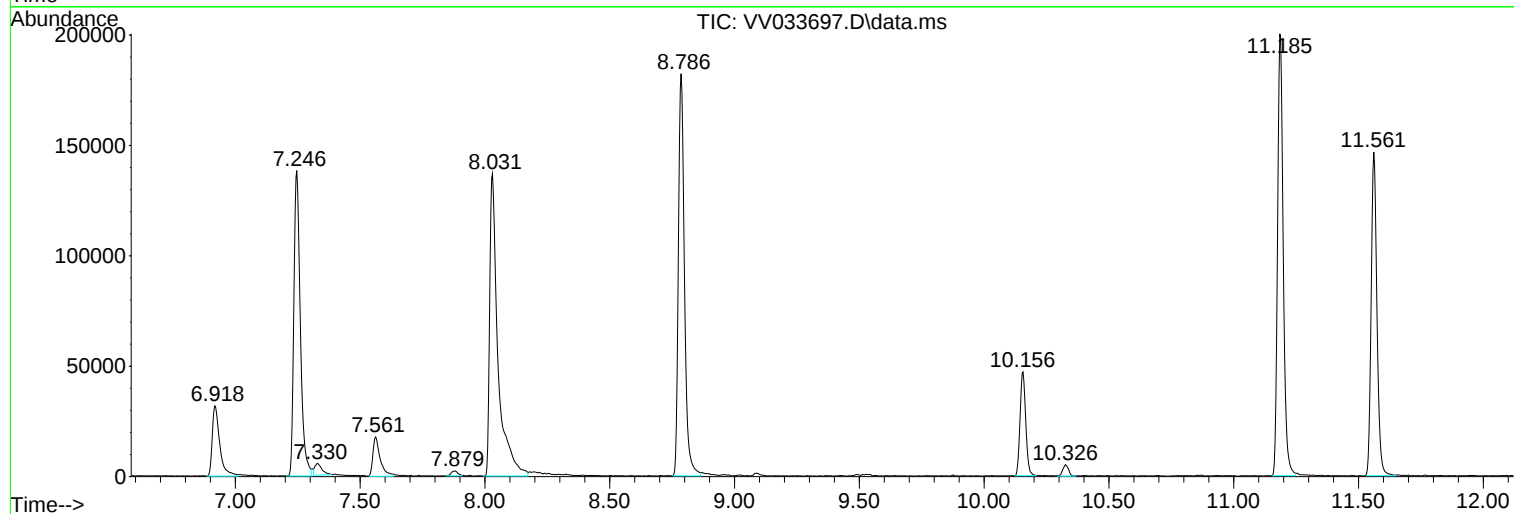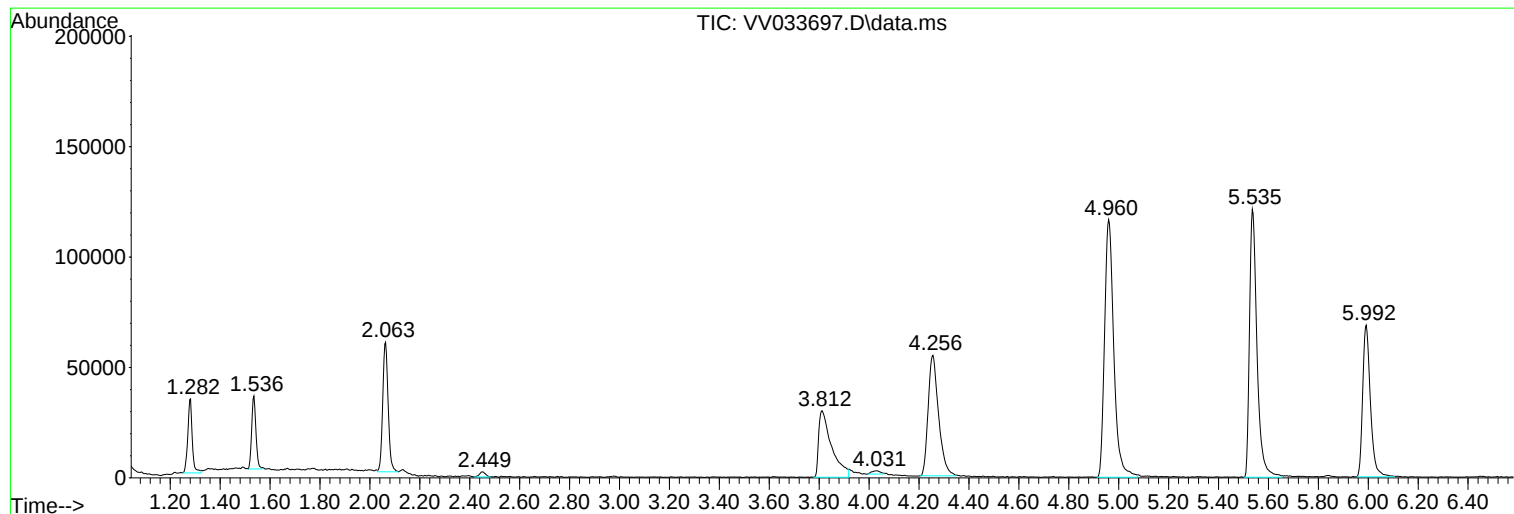

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033697.D
Acq On : 17 Jan 2024 02:08
Operator : SY/MD
Sample : P1143-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033697.D
Acq On : 17 Jan 2024 02:08
Operator : SY/MD
Sample : P1143-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc