


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV011624\
Data File : VV033655.D
Acq On : 16 Jan 2024 08:26
Operator : SY/MD
Sample : BFB239
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB239

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 18 00:02:20 2024

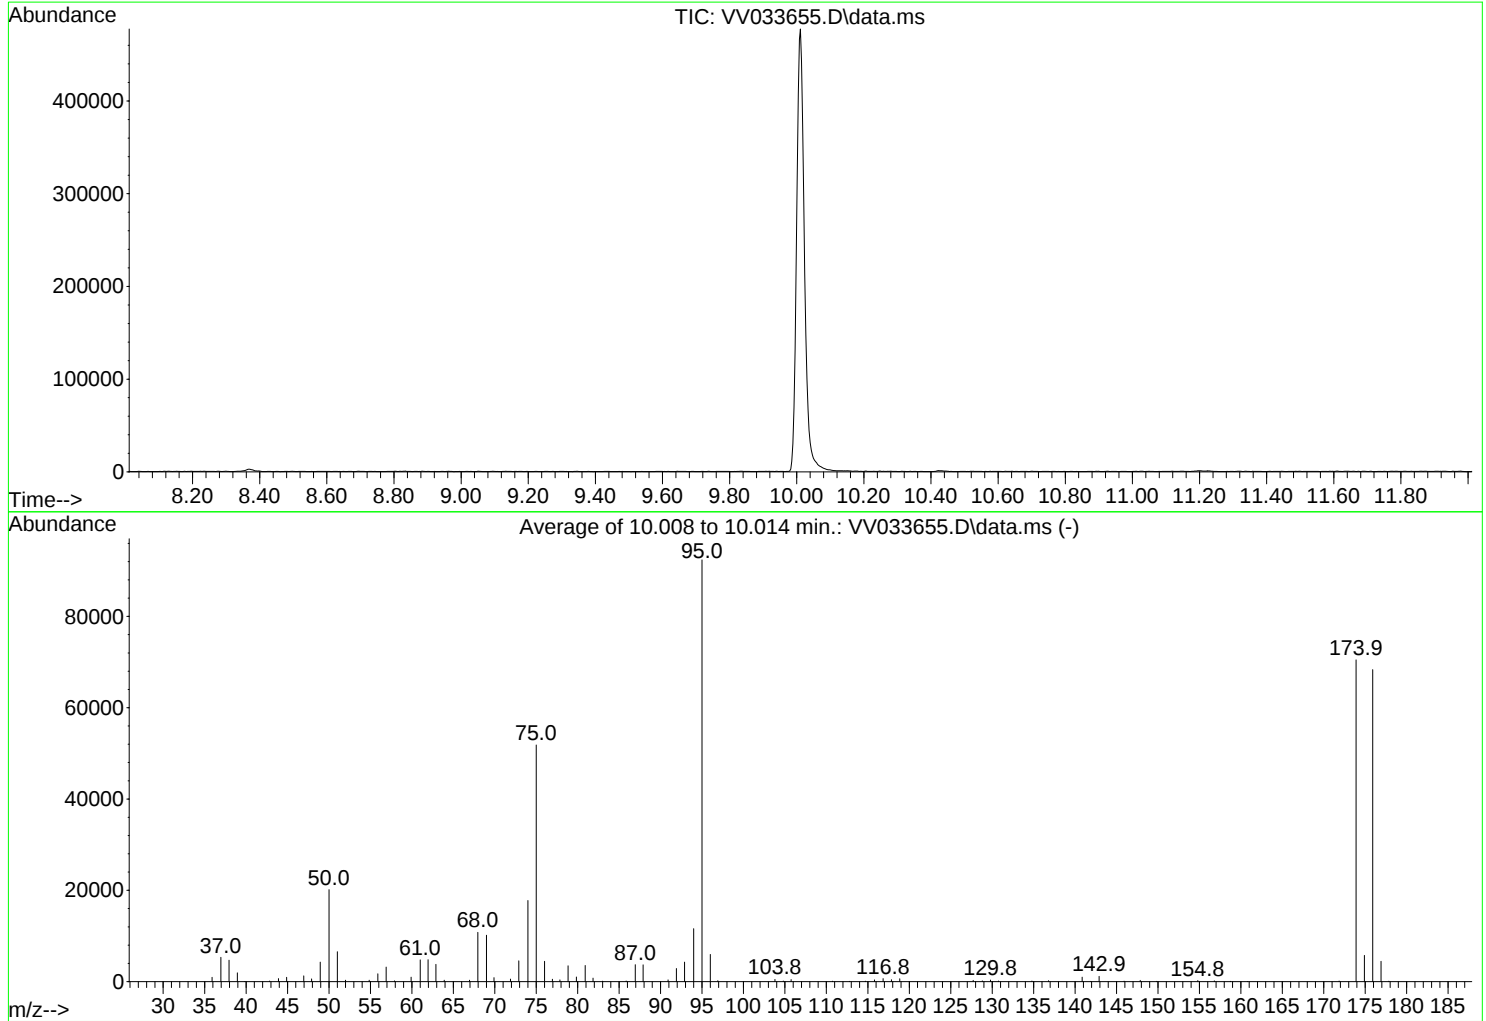

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.8	20147	PASS
75	95	30	80	56.1	51848	PASS
95	95	100	100	100.0	92389	PASS
96	95	5	9	6.4	5955	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.3	70499	PASS
175	174	5	9	8.2	5751	PASS
176	174	95	105	97.0	68352	PASS
177	176	5	10	6.5	4445	PASS

m/z	Abundance
39.80	151.0
40.90	109.0
43.90	238.0
77.10	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
35.90	1045.0
37.00	5478.0
37.90	4858.0
38.90	1913.0
39.90	191.0
42.80	139.0
43.90	924.0
44.90	965.0
46.90	1316.0
47.90	685.0
49.00	4338.0
50.00	20640.0
51.00	6854.0
52.00	298.0
54.80	372.0
55.90	1796.0
56.90	3249.0
57.90	157.0
59.90	993.0
61.00	4811.0
62.00	4971.0
62.90	3800.0
63.90	364.0
67.00	328.0
67.90	10994.0
69.00	10414.0
69.90	914.0
71.90	527.0
72.90	4858.0
74.00	18384.0
75.00	52944.0
76.00	4545.0
76.90	650.0
77.90	421.0
78.90	3541.0
79.90	1039.0
80.90	3616.0
81.90	753.0
83.00	106.0
85.90	126.0
86.90	3791.0
87.90	3634.0
90.90	359.0
91.90	2953.0
92.90	4361.0
94.00	11871.0
95.00	93936.0
96.00	6043.0
96.90	280.0
103.80	484.0
104.80	162.0
105.70	421.0
110.70	108.0
112.80	104.0
114.70	112.0
115.80	360.0
116.90	603.0
117.80	393.0
118.90	633.0
127.70	284.0
128.80	192.0
129.80	340.0
130.70	136.0
134.80	167.0
136.80	221.0
140.90	1002.0
141.90	126.0
142.90	1220.0
145.90	101.0
147.80	261.0
154.80	243.0
156.80	183.0
158.80	120.0
160.80	100.0
173.90	69552.0
174.90	5771.0
175.90	67048.0
176.90	4409.0
177.80	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
35.90	977.0
37.00	5472.0
38.00	4858.0
38.90	2030.0
39.90	211.0
42.80	140.0
43.90	906.0
44.90	980.0
46.90	1290.0
47.90	605.0
49.00	4385.0
50.00	20704.0
51.00	6798.0
52.00	325.0
54.80	327.0
55.90	1810.0
56.90	3318.0
57.90	166.0
59.90	1017.0
61.00	4920.0
62.00	5000.0
62.90	3895.0
63.90	315.0
67.00	319.0
68.00	11210.0
69.00	10497.0
69.90	881.0
71.90	607.0
72.90	4719.0
74.00	18544.0
75.00	53608.0
76.00	4587.0
76.90	662.0
77.90	409.0
78.90	3569.0
79.90	1055.0
80.90	3684.0
81.90	777.0
83.00	118.0
85.80	127.0
86.90	3858.0
87.90	3758.0
90.90	373.0
91.90	2983.0
92.90	4373.0
94.00	12025.0
95.00	95416.0
96.00	6106.0
96.90	227.0
103.80	525.0
104.80	169.0
105.70	454.0
110.70	123.0
112.80	102.0
114.70	114.0
115.80	382.0
116.80	690.0
117.90	444.0
118.80	646.0
127.70	296.0
128.80	185.0
129.80	349.0
130.70	163.0
134.80	144.0
136.80	234.0
140.90	1027.0
141.90	108.0
142.90	1217.0
145.90	106.0
147.90	271.0
149.80	101.0
154.80	233.0
156.80	198.0
158.70	120.0
171.90	209.0
173.90	72872.0
174.90	5967.0
175.90	70592.0
176.90	4531.0
177.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
35.90	830.0
36.90	5009.0
37.90	4389.0
39.00	1818.0
39.90	195.0
42.90	125.0
44.00	880.0
44.90	896.0
47.00	1173.0
47.90	476.0
48.90	4118.0
50.00	19096.0
51.00	6073.0
52.00	279.0
54.90	269.0
55.90	1584.0
56.90	3006.0
57.90	167.0
59.90	922.0
61.00	4564.0
61.90	4477.0
62.90	3648.0
63.90	262.0
66.90	310.0
67.90	10202.0
69.00	9630.0
69.90	802.0
71.90	585.0
72.90	4125.0
74.00	16416.0
75.00	48992.0
76.00	4177.0
77.00	605.0
77.80	362.0
78.80	3263.0
79.80	984.0
80.90	3343.0
81.80	786.0
83.00	124.0
85.80	122.0
87.00	3522.0
87.90	3688.0
90.90	386.0
91.90	2674.0
92.90	4084.0
94.00	10868.0
95.00	87816.0
96.00	5715.0
96.90	170.0
103.80	511.0
104.80	141.0
105.80	459.0
110.80	125.0
114.70	103.0
115.80	383.0
116.80	700.0
117.90	432.0
118.80	587.0
127.70	310.0
128.80	178.0
129.80	352.0
130.80	179.0
134.80	131.0
136.80	206.0
140.80	916.0
142.90	1071.0
145.90	115.0
147.90	260.0
149.90	114.0
154.80	221.0
156.80	187.0
171.80	227.0
173.90	69072.0
174.90	5515.0
175.90	67416.0
176.90	4396.0
177.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239