

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050922\
 Data File : VV025853.D
 Acq On : 09 May 2022 11:52
 Operator : SY/MD
 Sample : N2678-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: May 10 04:47:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 10 04:47:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	205166	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	212848	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	95179	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	85149	3.786	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.800%
7) Chloroethane-d5	1.568	69	87994	4.448	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.000%
11) 1,1-Dichloroethene-d2	2.104	63	139344	3.262	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.200%
20) 2-Butanone-d5	3.895	46	166948	54.246	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.500%
24) Chloroform-d	4.342	84	165281	4.907	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.027	65	78985	5.298	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.000%
32) Benzene-d6	5.043	84	315944	4.622	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
36) 1,2-Dichloropropane-d6	6.066	67	98992	4.924	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%
41) Toluene-d8	7.313	98	259666	4.199	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.000%
43) trans-1,3-Dichloroprop...	7.619	79	28759	4.519	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%
46) 2-Hexanone-d5	8.088	63	134341	54.165	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.340%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	64696	5.097	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	90904	5.445	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.800%
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	4497	0.234	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050922\
Data File : VV025853.D
Acq On : 09 May 2022 11:52
Operator : SY/MD
Sample : N2678-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: May 10 04:47:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 10 04:47:02 2022
Response via : Initial Calibration

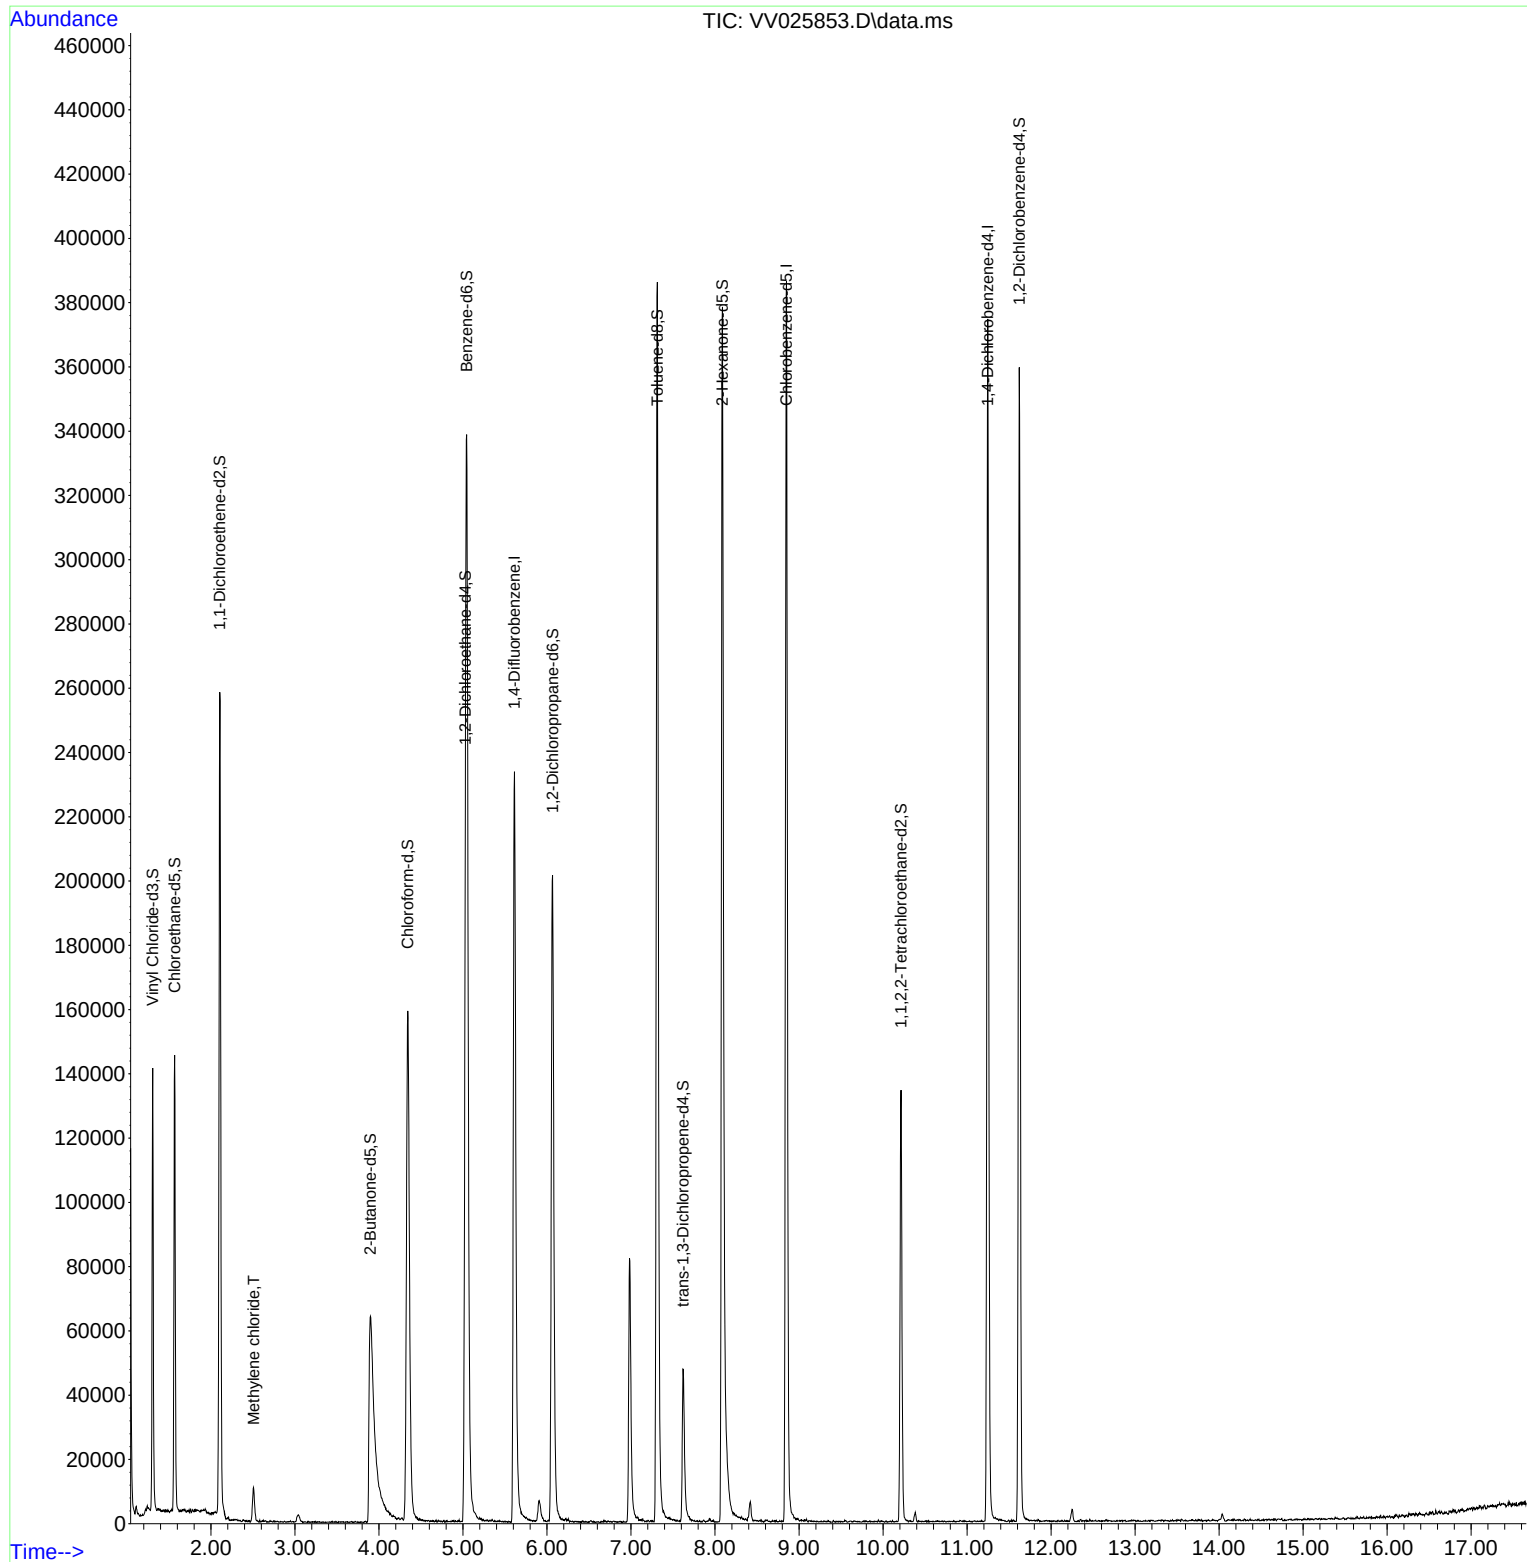

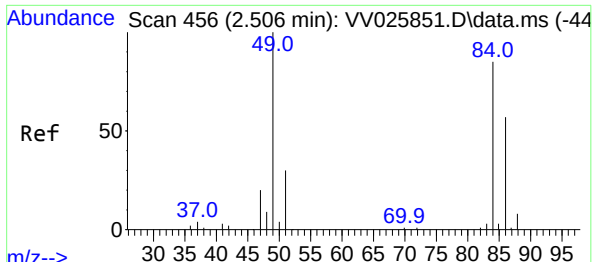

#16
Methylene chloride
Concen: 0.234 ug/L
RT: 2.506 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV025853.D
Acq: 09 May 2022 11:52

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

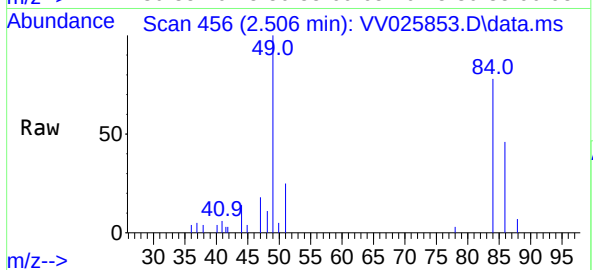

Tgt Ion: 84 Resp: 4497

Ion	Ratio	Lower	Upper
84	100		
86	59.9	45.9	85.3
49	129.0	76.6	142.3

