

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050922\
 Data File : VV025852.D
 Acq On : 09 May 2022 10:47
 Operator : SY/MD
 Sample : VV0509WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK358

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	100	rVB	116905	125057	16.37%	2.063%
2	1.568	157	164	179	rVB	124567	142577	18.66%	2.352%
3	2.105	321	331	346	rVB	237200	334424	43.77%	5.518%
4	2.506	443	456	468	rBV3	7172	12843	1.68%	0.212%
5	3.899	878	889	918	rBV2	59473	242622	31.76%	4.003%
6	4.342	1010	1027	1053	rBV	137798	353370	46.25%	5.830%
7	5.043	1229	1245	1275	rBV2	303476	764015	100.00%	12.606%
8	5.612	1410	1422	1449	rBV	221725	454216	59.45%	7.494%
9	5.905	1503	1513	1527	rBV8	5917	12647	1.66%	0.209%
10	6.066	1549	1563	1593	rBV2	179607	377648	49.43%	6.231%
11	6.985	1838	1849	1877	rBV	70669	136697	17.89%	2.255%
12	7.313	1938	1951	1975	rBV	336076	591868	77.47%	9.765%
13	7.622	2035	2047	2070	rBV	40744	77569	10.15%	1.280%
14	8.088	2181	2192	2232	rBV	336954	657047	86.00%	10.841%
15	8.416	2283	2294	2307	rVB4	4286	8446	1.11%	0.139%
16	8.850	2418	2429	2448	rBV	357032	580802	76.02%	9.583%
17	10.214	2842	2853	2870	rBV2	117061	186313	24.39%	3.074%
18	11.246	3163	3174	3195	rBV	333731	518326	67.84%	8.552%
19	11.622	3279	3291	3313	rBV	308443	484422	63.40%	7.993%




Sum of corrected areas: 6060909

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050922\
Data File : VV025852.D
Acq On : 09 May 2022 10:47
Operator : SY/MD
Sample : VV0509WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

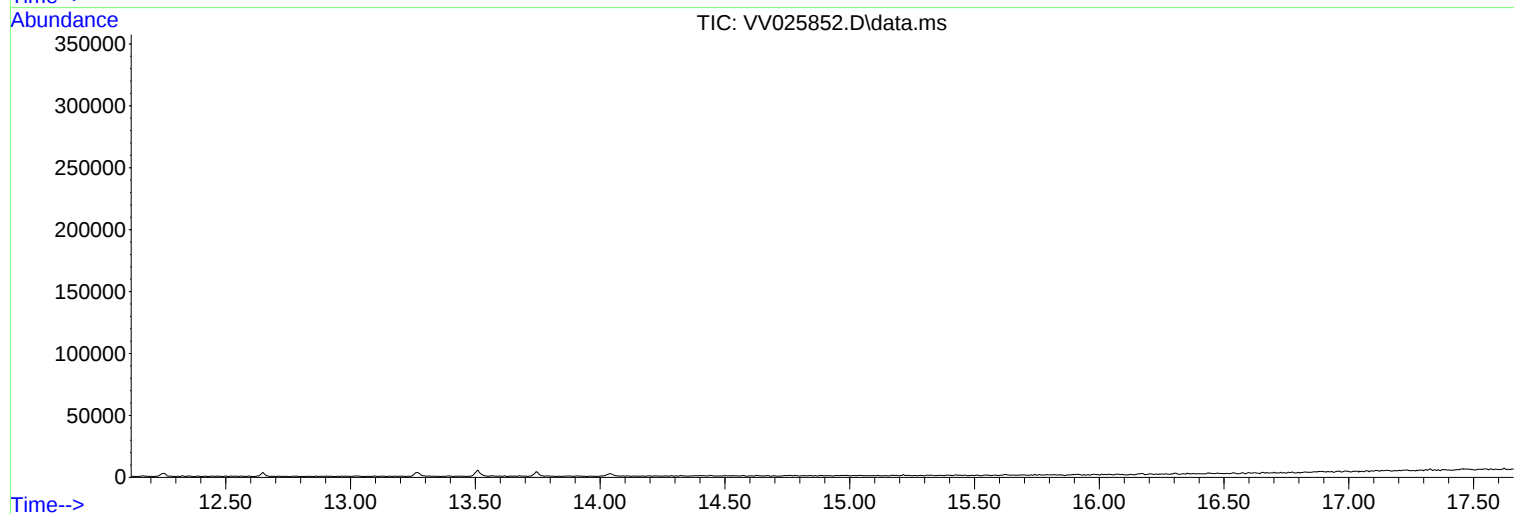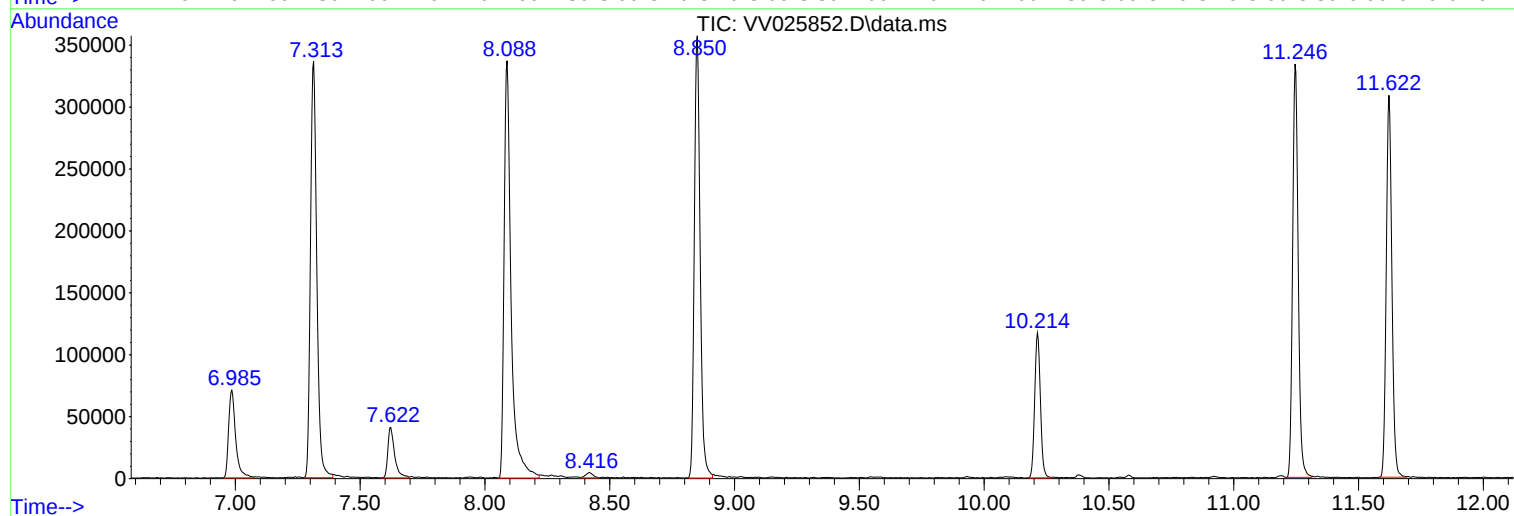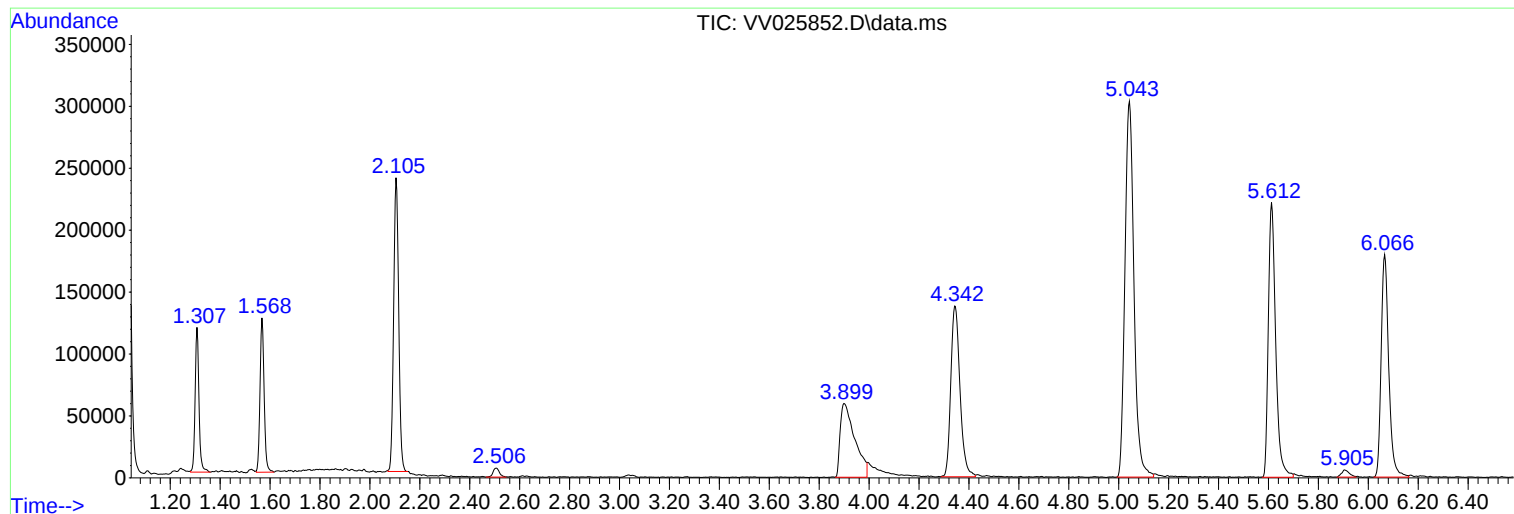

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050922\
Data File : VV025852.D
Acq On : 09 May 2022 10:47
Operator : SY/MD
Sample : VV0509WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050922\
Data File : VV025852.D
Acq On : 09 May 2022 10:47
Operator : SY/MD
Sample : VV0509WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc