
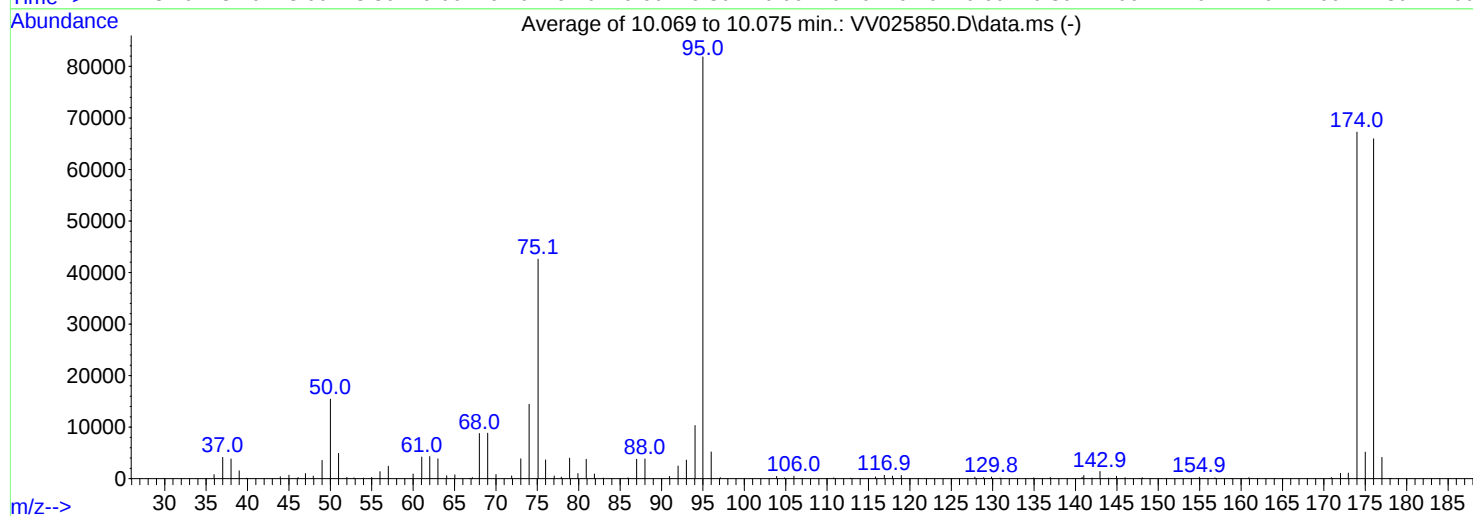


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050922\
 Data File : VV025850.D
 Acq On : 09 May 2022 09:39
 Operator : SY/MD
 Sample : BFB315
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB315

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue May 10 04:47:02 2022

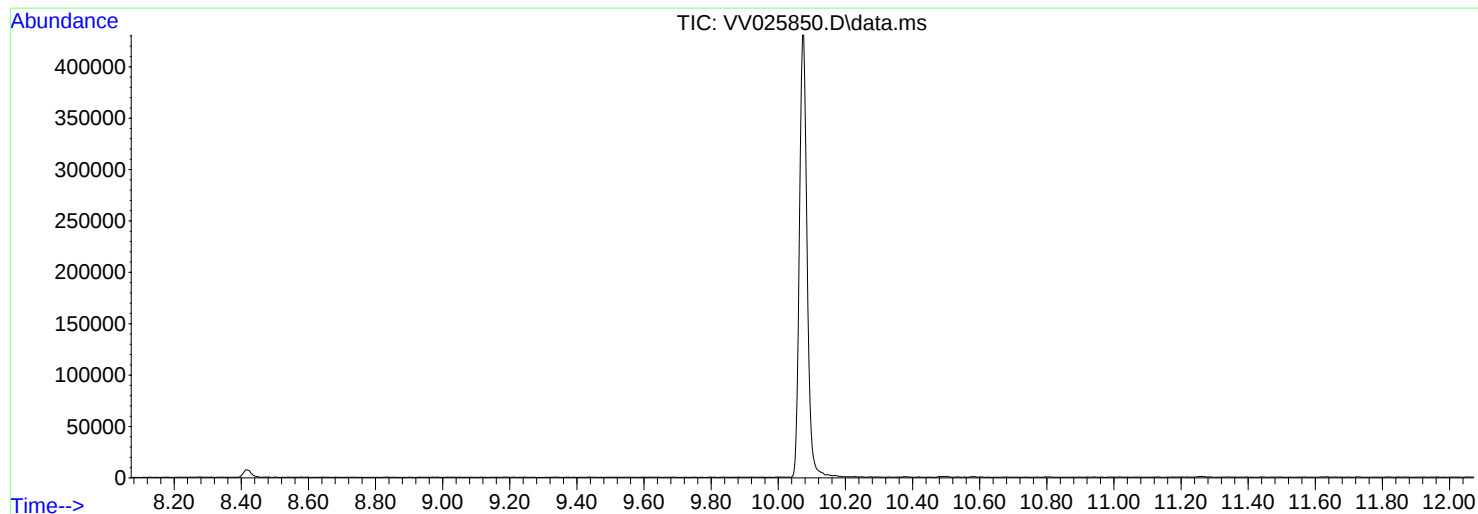

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	15428	PASS
75	95	30	80	52.0	42592	PASS
95	95	100	100	100.0	81851	PASS
96	95	5	9	6.3	5190	PASS
173	174	0.00	2	1.6	1101	PASS
174	95	50	120	82.2	67251	PASS
175	174	5	9	7.7	5145	PASS
176	174	95	105	98.1	65963	PASS
177	176	5	10	6.3	4145	PASS

Scan 2796 (10.030 min): VV025850.D\data.ms
BFB315

m/z	Abundance
39.90	233.0
43.90	515.0

Instrument :
MSVOA_V
ClientSampleId :
BFB315

m/z	Abundance
36.00	744.0
37.00	3911.0
38.00	3643.0
39.00	1483.0
39.90	356.0
44.00	822.0
45.00	552.0
46.20	184.0
47.00	931.0
47.90	486.0
49.00	3383.0
50.00	14586.0
51.00	4667.0
52.00	270.0
52.80	188.0
54.00	112.0
55.00	272.0
56.00	1251.0
57.00	2337.0
60.00	824.0
61.00	3954.0
62.00	4016.0
63.00	3744.0
64.00	572.0
65.10	684.0
66.80	205.0
67.20	187.0
68.00	8308.0
69.00	8519.0
70.00	726.0
71.90	552.0
73.00	3675.0
74.00	14027.0
75.10	40224.0
76.00	3490.0
77.00	552.0
77.90	343.0
78.90	3773.0
79.90	868.0
80.90	3656.0
81.90	848.0
82.90	110.0
86.00	160.0
87.00	3640.0
88.00	3562.0
91.00	416.0
92.00	2192.0
93.00	3257.0
94.10	9737.0
95.00	76808.0
96.00	4985.0
97.10	171.0
103.90	432.0
104.90	119.0
106.00	454.0
110.00	106.0
110.80	137.0
112.80	160.0
115.90	336.0
116.90	632.0
117.90	416.0
119.00	678.0
127.80	285.0
128.90	234.0
129.80	323.0
130.90	136.0
135.00	148.0
137.00	207.0
140.80	827.0
142.10	137.0
143.00	1332.0
144.00	113.0
145.00	422.0
146.00	161.0
147.70	151.0
148.10	152.0
155.00	201.0
156.90	155.0
160.90	152.0
171.10	171.0
172.00	906.0
173.00	1054.0
174.00	61000.0
175.00	4689.0
176.00	59840.0
177.00	3871.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB315

m/z	Abundance
36.00	794.0
37.00	4321.0
38.00	3995.0
39.00	1570.0
39.90	331.0
44.00	904.0
45.00	733.0
46.10	245.0
47.00	1026.0
48.00	508.0
49.00	3620.0
50.00	15973.0
51.00	5056.0
52.00	259.0
52.80	172.0
54.00	117.0
55.00	265.0
56.00	1435.0
57.00	2526.0
60.00	972.0
61.00	4290.0
62.00	4394.0
63.00	3923.0
64.00	579.0
65.00	767.0
67.20	222.0
68.00	9066.0
69.00	9102.0
70.00	824.0
71.90	554.0
73.00	3996.0
74.00	14866.0
75.10	44024.0
76.00	3719.0
77.10	543.0
77.90	310.0
78.90	4093.0
79.90	1018.0
80.90	3911.0
81.90	941.0
83.00	147.0
85.90	183.0
87.00	3918.0
88.00	3960.0
91.00	451.0
92.00	2511.0
93.00	3699.0
94.10	10627.0
95.00	84952.0
96.00	5280.0
97.10	216.0
103.90	476.0
104.80	135.0
106.00	502.0
110.80	163.0
112.90	131.0
115.80	357.0
116.90	697.0
117.90	556.0
119.00	656.0
127.90	318.0
128.90	244.0
129.80	342.0
130.90	140.0
134.90	180.0
137.00	218.0
141.00	909.0
142.00	121.0
143.00	1443.0
144.00	116.0
144.90	481.0
146.00	174.0
148.00	189.0
154.90	272.0
156.80	157.0
160.90	189.0
170.90	218.0
172.00	1086.0
172.90	1137.0
174.00	69448.0
175.00	5364.0
176.00	68304.0
177.00	4213.0
177.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB315

m/z	Abundance
35.90	772.0
37.00	4206.0
38.00	3833.0
39.00	1507.0
40.00	312.0
44.00	902.0
45.00	797.0
46.00	267.0
47.00	1070.0
48.00	485.0
49.00	3636.0
50.00	15726.0
51.00	5017.0
52.00	235.0
52.90	154.0
54.00	117.0
55.00	215.0
56.00	1459.0
57.00	2420.0
60.00	918.0
61.10	4390.0
62.00	4443.0
63.00	3866.0
64.10	558.0
65.00	819.0
67.10	244.0
68.00	8894.0
69.00	8856.0
70.00	851.0
71.90	477.0
73.00	3855.0
74.00	14418.0
75.10	43528.0
76.00	3652.0
77.10	513.0
77.90	273.0
78.90	4039.0
79.90	1080.0
80.90	3747.0
81.90	927.0
83.00	169.0
85.90	165.0
87.00	3749.0
88.00	3926.0
90.90	406.0
92.00	2635.0
93.00	3861.0
94.00	10552.0
95.00	83792.0
96.00	5306.0
97.10	221.0
103.90	439.0
104.80	182.0
106.00	500.0
106.80	117.0
110.80	152.0
115.80	355.0
116.90	663.0
117.90	526.0
118.90	575.0
127.90	310.0
128.90	214.0
129.90	312.0
130.90	115.0
134.90	177.0
136.90	207.0
139.70	110.0
141.00	936.0
141.90	121.0
142.90	1412.0
144.00	114.0
144.90	470.0
146.00	185.0
148.00	236.0
154.90	334.0
156.80	152.0
158.80	115.0
161.00	207.0
170.80	247.0
172.00	1112.0
172.90	1111.0
174.00	71304.0
175.00	5383.0
176.00	69744.0
177.00	4350.0
178.10	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB315