

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051322\
 Data File : VV025896.D
 Acq On : 13 May 2022 18:29
 Operator : SY/MD
 Sample : VIBLK249
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK249

Quant Time: May 14 07:23:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 14 07:17:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	153467	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	157036	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70052	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	64017	5.051	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.000%
7) Chloroethane-d5	1.571	69	57415	5.290	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.800%
11) 1,1-Dichloroethene-d2	2.108	63	100156	3.570	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.400%
20) 2-Butanone-d5	3.902	46	50251	34.234	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	68.460%
24) Chloroform-d	4.346	84	103447	4.997	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	5.034	65	44522	5.071	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.400%
32) Benzene-d6	5.050	84	209659	5.141	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.800%
36) 1,2-Dichloropropane-d6	6.069	67	62607	5.281	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.600%
41) Toluene-d8	7.313	98	178752	4.715	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
43) trans-1,3-Dichloroprop...	7.625	79	17941	4.627	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.600%
46) 2-Hexanone-d5	8.088	63	60069	41.727	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.460%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	34439	4.510	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	54395	5.454	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.000%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	5693	0.380	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051322\
Data File : VV025896.D
Acq On : 13 May 2022 18:29
Operator : SY/MD
Sample : VIBLK249
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK249

Quant Time: May 14 07:23:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 14 07:17:53 2022
Response via : Initial Calibration

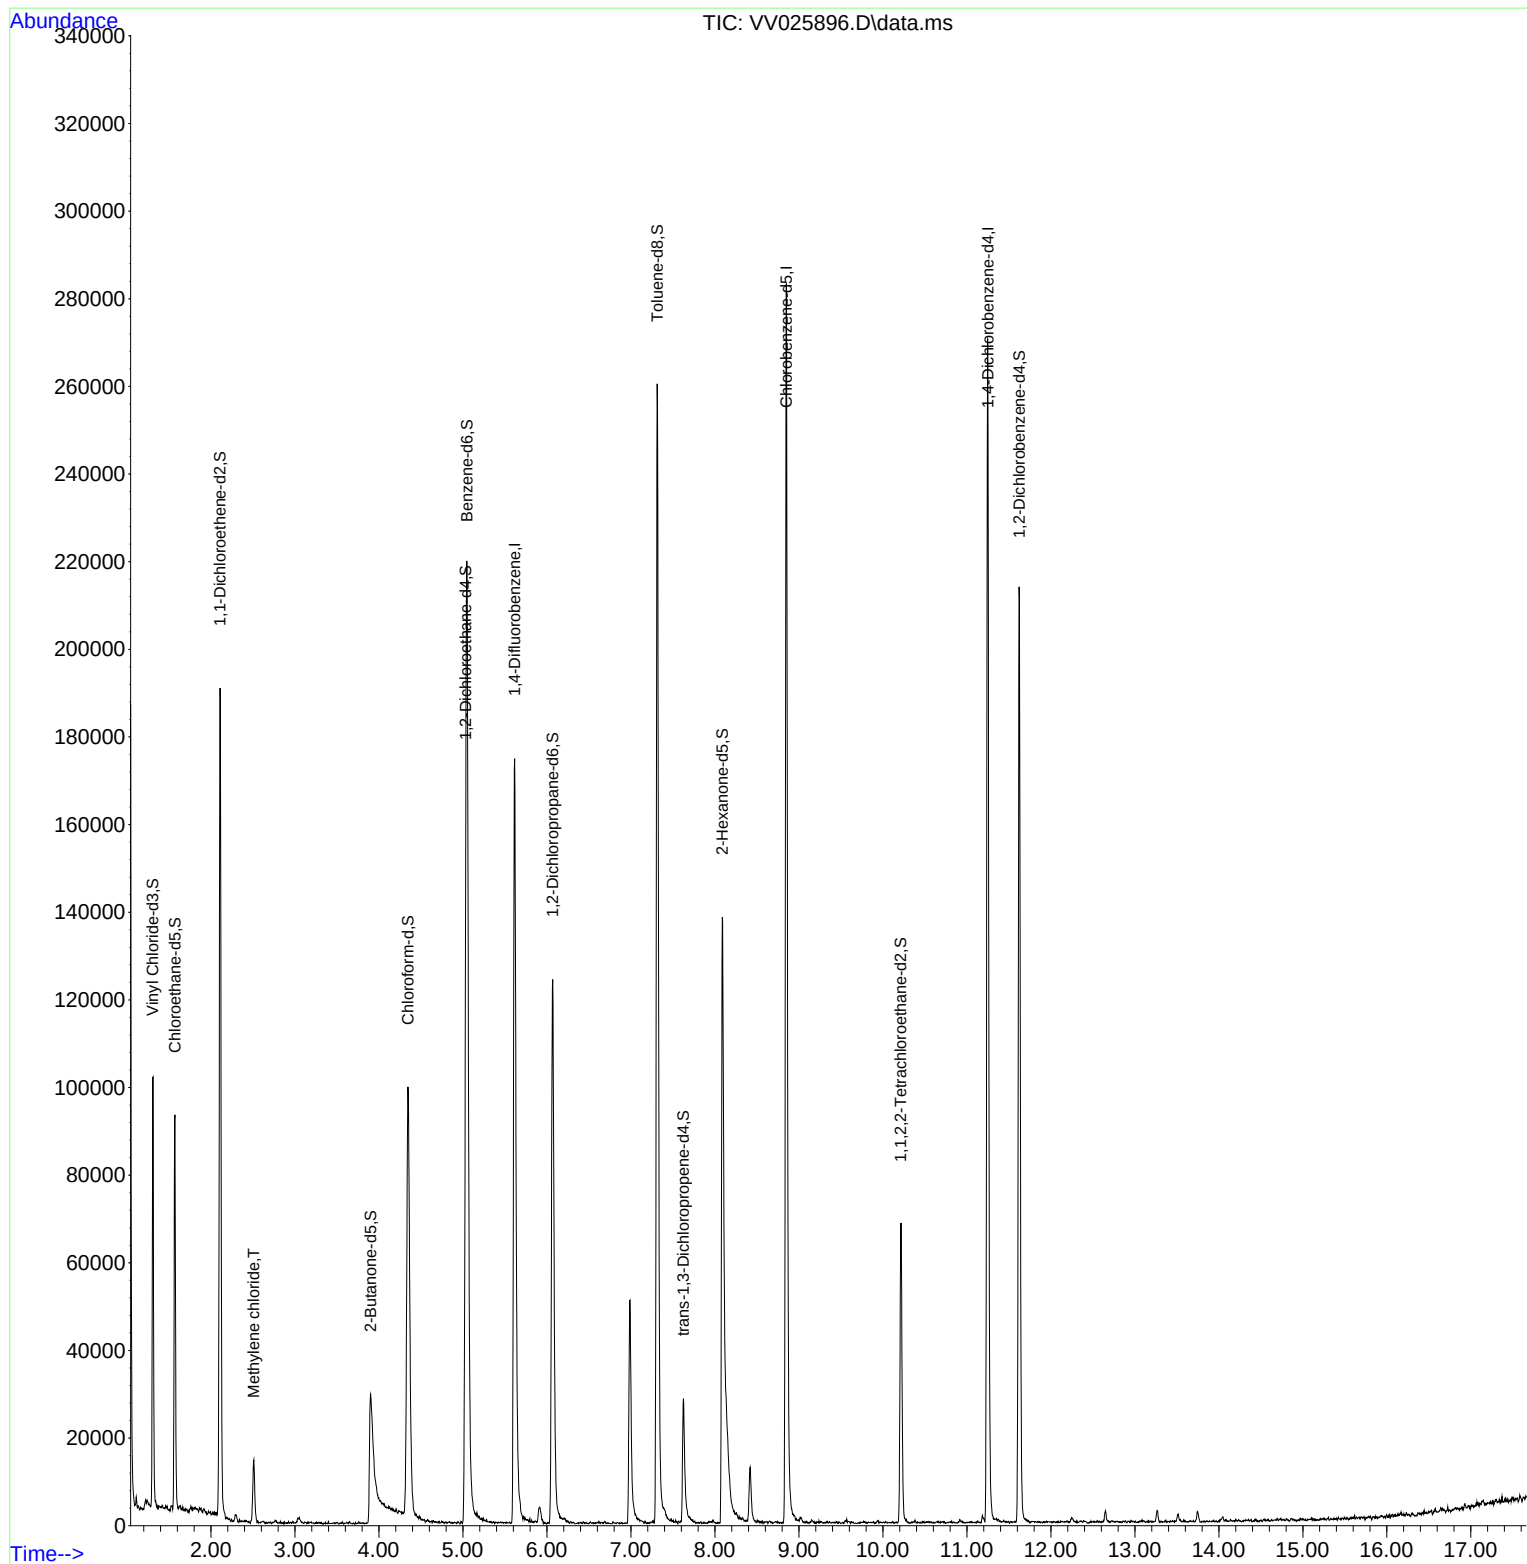

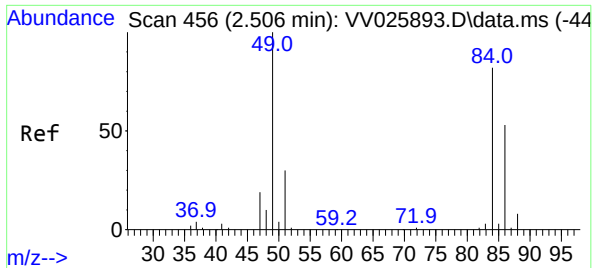

#16
Methylene chloride
Concen: 0.380 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025896.D
Acq: 13 May 2022 18:29

Instrument :
MSVOA_V
ClientSampleId :
VIBLK249

Tgt Ion: 84 Resp: 5693
Ion Ratio Lower Upper
84 100
86 55.7 45.4 84.2
49 108.7 85.6 159.0

