


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051322\
 Data File : VV025889.D
 Acq On : 13 May 2022 10:38
 Operator : SY/MD
 Sample : BFB316
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB316

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue May 17 07:58:29 2022

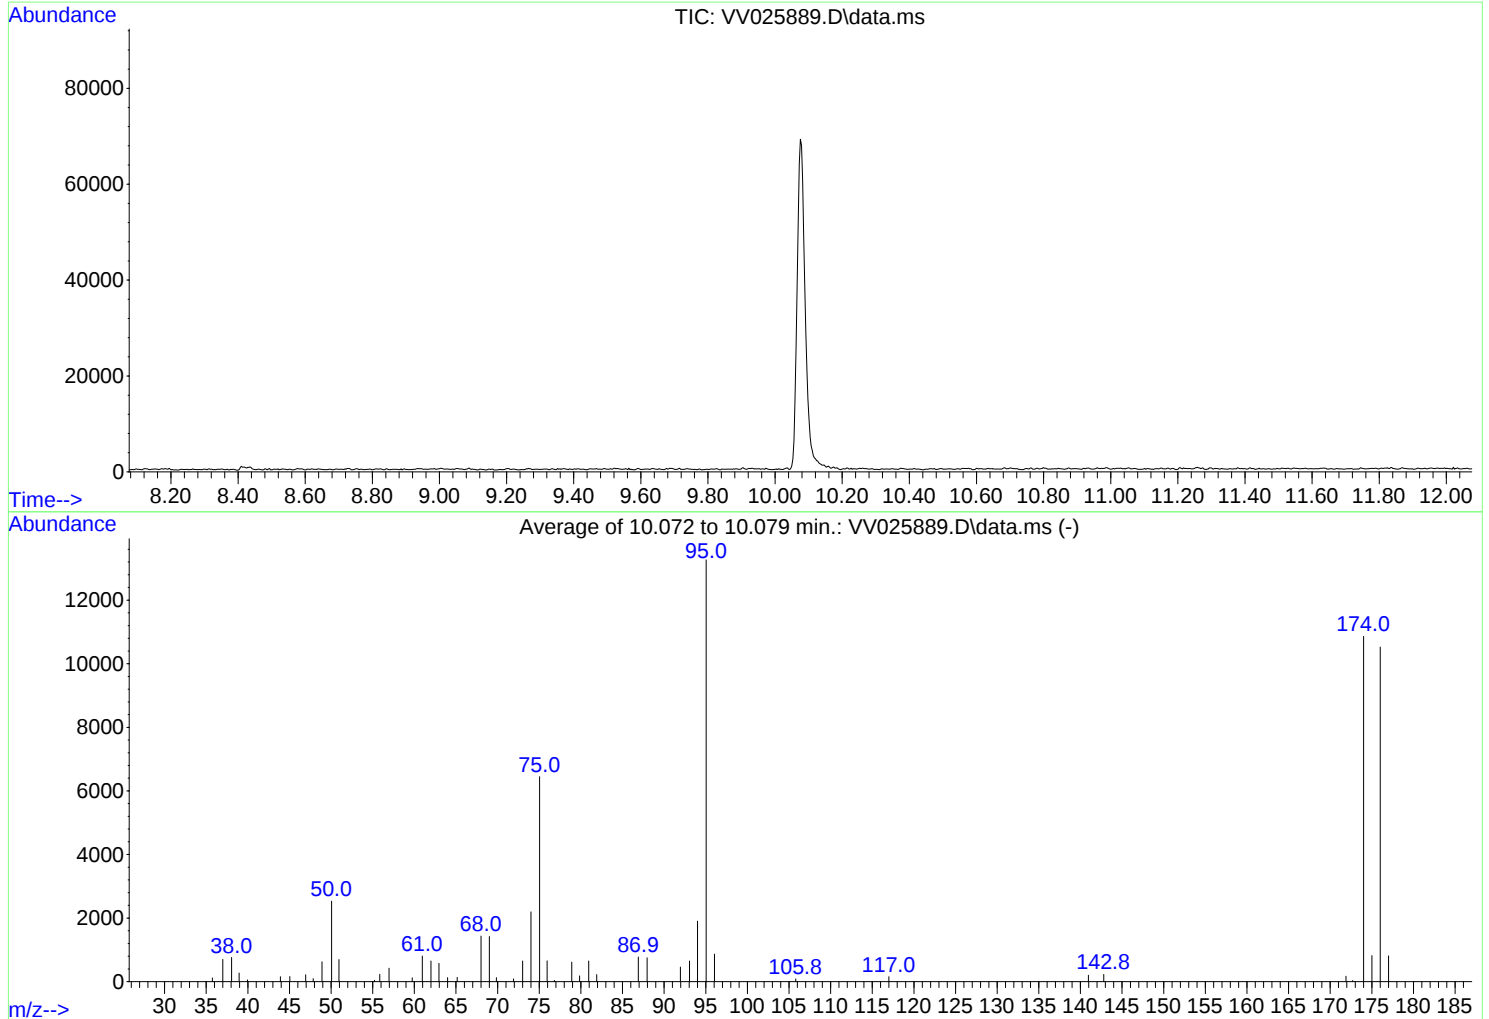

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	2534	PASS
75	95	30	80	48.6	6447	PASS
95	95	100	100	100.0	13269	PASS
96	95	5	9	6.5	868	PASS
173	174	0.00	2	0.3	36	PASS
174	95	50	120	81.9	10864	PASS
175	174	5	9	7.6	821	PASS
176	174	95	105	96.9	10523	PASS
177	176	5	10	7.7	808	PASS

Scan 2799 (10.040 min): VV025889.D\data.ms
BFB316

m/z	Abundance
36.40	106.0
39.90	213.0
43.90	259.0

Instrument :
MSVOA_V
ClientSampleId :
BFB316

m/z	Abundance
35.70	105.0
37.00	746.0
38.10	740.0
39.00	275.0
40.10	233.0
43.90	354.0
45.10	148.0
46.90	171.0
48.90	641.0
50.00	2543.0
50.90	645.0
55.20	116.0
55.90	240.0
56.90	418.0
59.80	118.0
61.00	839.0
62.00	623.0
63.00	610.0
65.20	126.0
68.00	1269.0
69.00	1471.0
69.80	116.0
73.00	602.0
74.00	2180.0
75.10	6027.0
76.00	577.0
78.90	542.0
79.90	193.0
80.90	670.0
81.90	199.0
86.90	776.0
88.00	651.0
92.00	434.0
93.10	649.0
94.00	1824.0
95.00	12621.0
96.10	903.0
117.00	135.0
140.90	227.0
142.80	219.0
171.90	173.0
172.70	108.0
174.00	10585.0
175.00	716.0
176.00	9865.0
177.00	817.0

Instrument :
MSVOA_V
ClientSampleId :
BFB316

m/z	Abundance
35.70	114.0
37.00	700.0
38.10	811.0
38.90	281.0
40.00	265.0
44.00	421.0
45.00	172.0
47.00	227.0
47.90	129.0
48.90	629.0
50.00	2609.0
51.00	692.0
55.90	239.0
57.00	433.0
59.80	135.0
61.00	857.0
62.00	637.0
63.00	591.0
64.00	147.0
65.20	141.0
68.00	1468.0
69.00	1463.0
69.80	135.0
71.90	110.0
73.00	675.0
74.00	2271.0
75.00	6627.0
75.90	667.0
78.90	649.0
79.80	188.0
80.90	667.0
81.90	228.0
86.90	818.0
87.90	823.0
92.00	457.0
93.10	662.0
94.00	1981.0
95.10	13753.0
96.00	894.0
105.80	115.0
117.00	164.0
140.90	211.0
142.80	239.0
171.90	167.0
174.00	11144.0
175.00	853.0
176.00	10884.0
177.00	830.0

Instrument :
MSVOA_V
ClientSampleId :
BFB316

m/z	Abundance
35.80	136.0
37.00	648.0
38.00	726.0
38.90	266.0
39.90	302.0
44.00	467.0
45.00	164.0
47.00	255.0
47.80	154.0
48.90	607.0
50.10	2451.0
51.00	743.0
55.80	220.0
57.00	416.0
59.70	117.0
60.90	721.0
62.00	687.0
62.90	514.0
64.00	228.0
65.00	143.0
68.00	1569.0
69.00	1326.0
69.90	127.0
71.90	149.0
73.00	663.0
74.00	2130.0
75.00	6686.0
75.90	714.0
76.80	118.0
78.90	652.0
79.80	169.0
81.00	611.0
81.90	233.0
86.90	738.0
87.90	780.0
91.90	477.0
93.00	635.0
94.00	1902.0
95.10	13433.0
96.00	808.0
105.80	139.0
117.00	166.0
141.00	165.0
142.80	226.0
171.90	171.0
174.00	10863.0
175.00	894.0
176.00	10820.0
177.00	776.0

Instrument :
MSVOA_V
ClientSampleId :
BFB316