




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025941.D
 Acq On : 20 May 2022 13:20
 Operator : SY/MD
 Sample : N2955-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA0

Manual IntegrationsAPPROVED

Quant Time: May 20 21:50:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 20 21:49:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/24/2022
 Supervised By :Mahesh Dadoda 05/24/2022

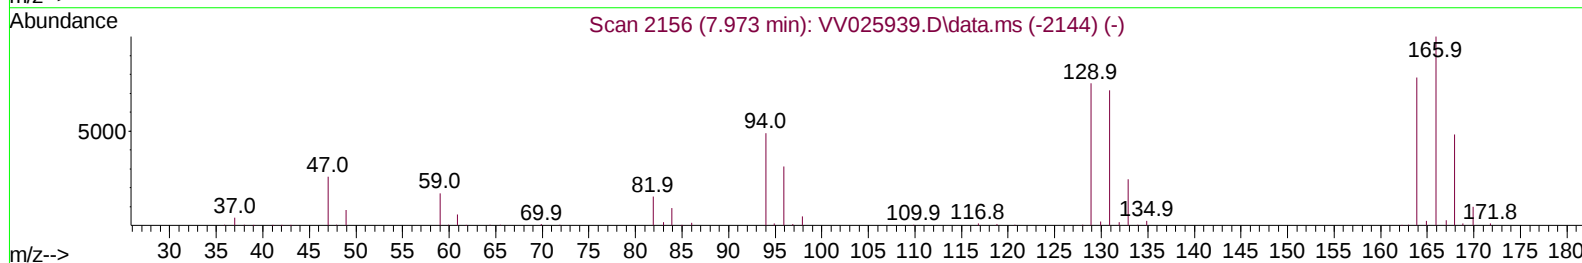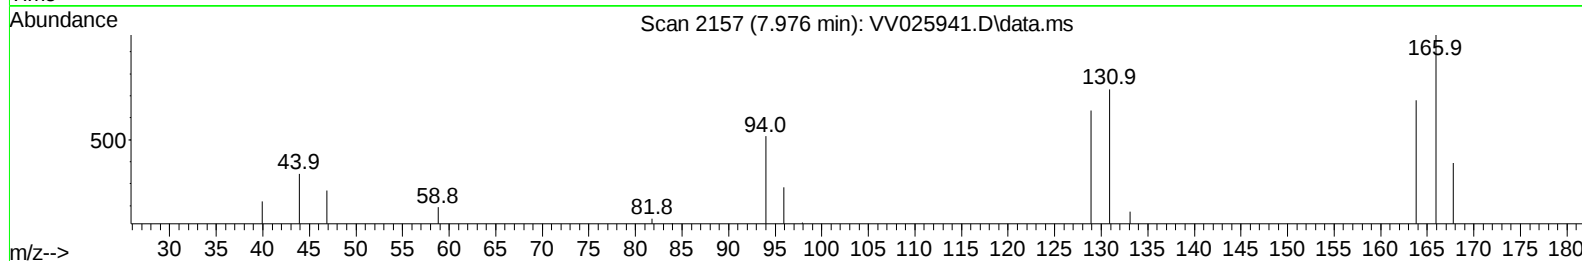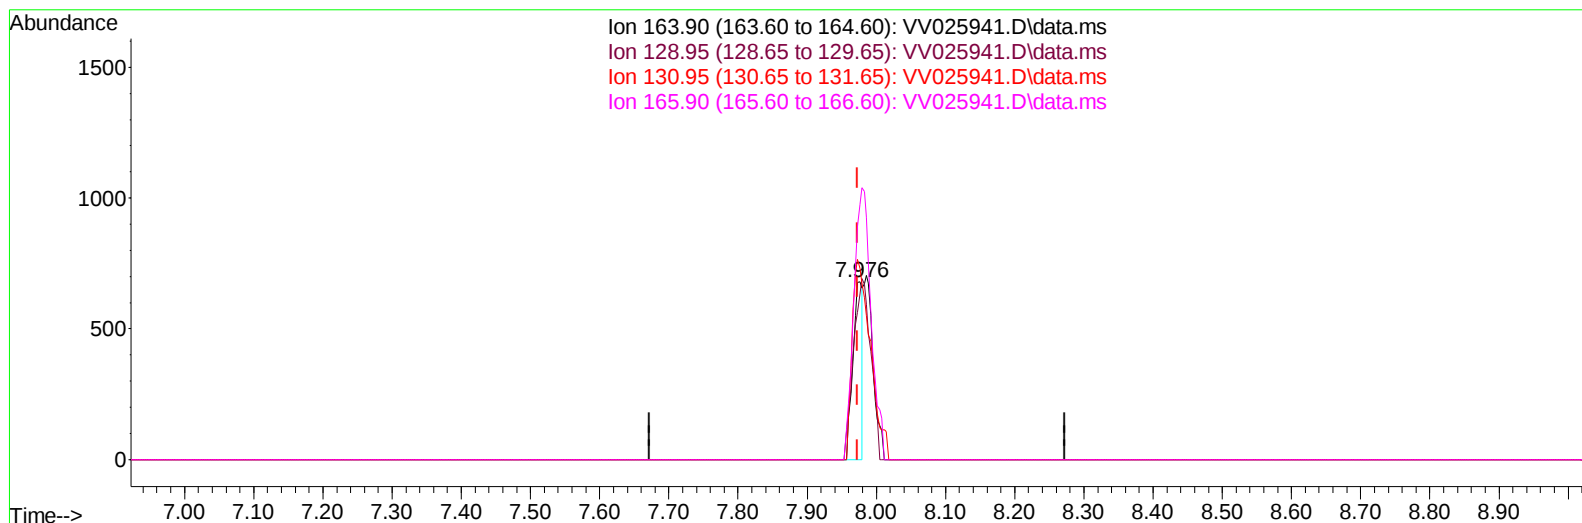

TIC: VV025941.D\data.ms

(47) Tetrachloroethene (T)

7.976min (+ 0.003) 0.06 ug/L

response 646

Ion	Exp%	Act%
163.90	100.00	100.00
128.95	96.50	93.08
130.95	91.10	107.51
165.90	124.10	143.74




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025941.D
 Acq On : 20 May 2022 13:20
 Operator : SY/MD
 Sample : N2955-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA0

Manual IntegrationsAPPROVED

Quant Time: May 20 21:50:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 20 21:49:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/24/2022
 Supervised By :Mahesh Dadoda 05/24/2022

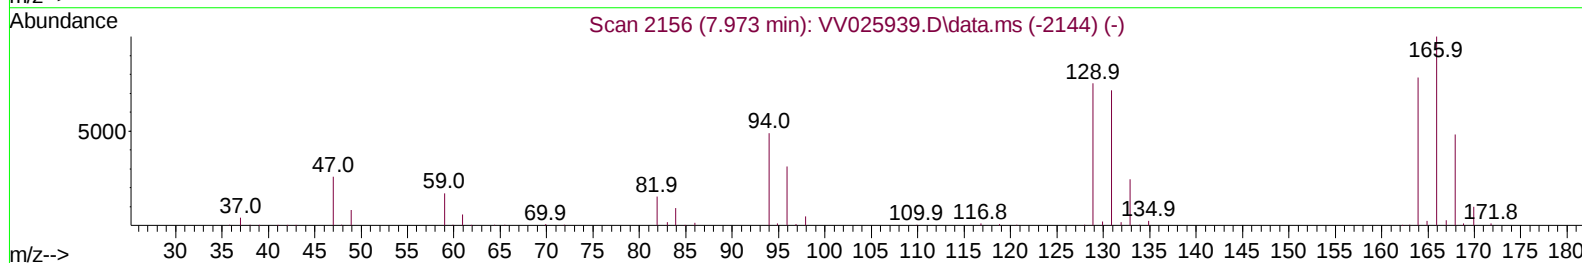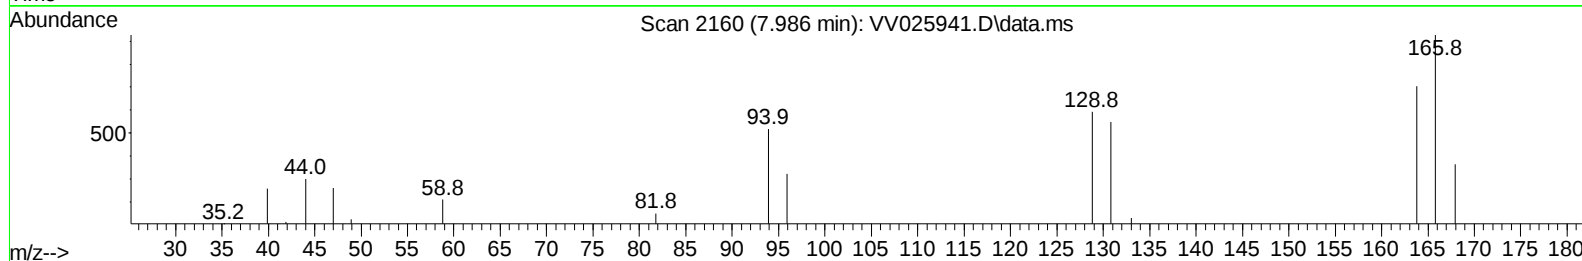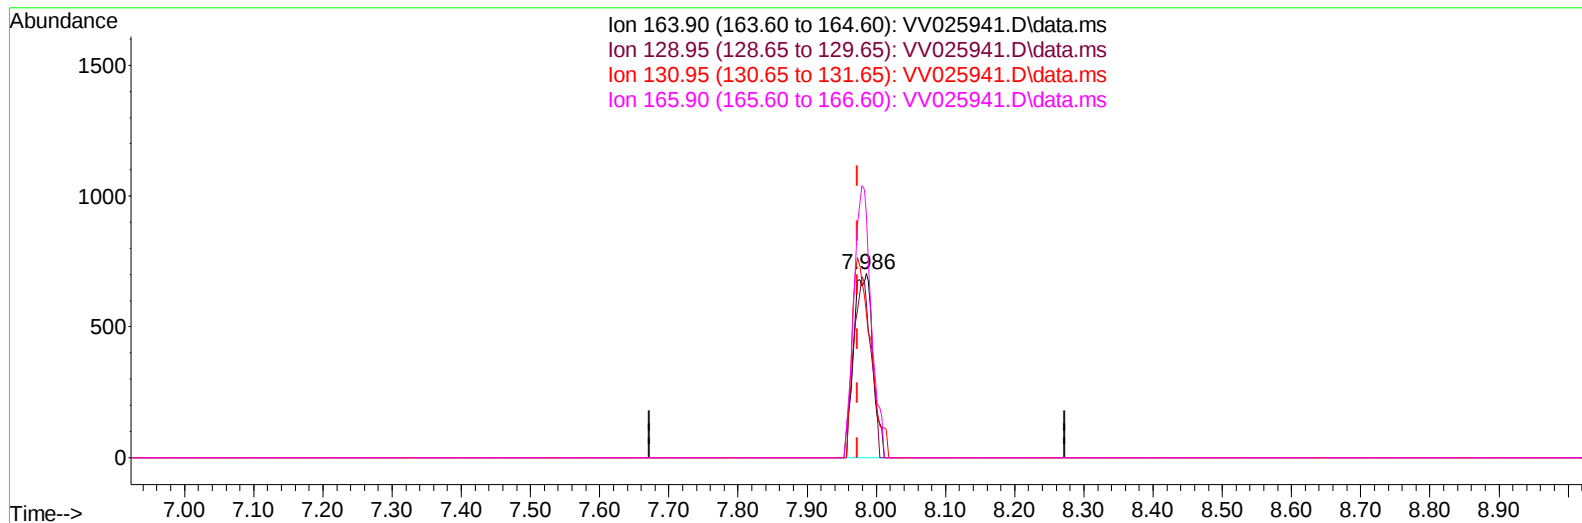

TIC: VV025941.D\data.ms

(47) Tetrachloroethene (T)

7.986min (+ 0.013) 0.11 ug/L m

response 1338

Ion	Exp%	Act%
163.90	100.00	100.00
128.95	96.50	84.23
130.95	91.10	77.98
165.90	124.10	131.68

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025941.D
 Acq On : 20 May 2022 13:20
 Operator : SY/MD
 Sample : N2955-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA0

Manual IntegrationsAPPROVED

Quant Time: May 20 21:50:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 20 21:49:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/24/2022
 Supervised By :Mahesh Dadoda 05/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	163500	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	174556	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76674	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	60337	4.468	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	89.400%	
7) Chloroethane-d5	1.571	69	59551	5.150	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	103.000%	
11) 1,1-Dichloroethene-d2	2.111	63	100734	3.370	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	67.400%	
20) 2-Butanone-d5	3.902	46	61127	39.088	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	78.180%	
24) Chloroform-d	4.349	84	126069	5.716	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	114.400%	
26) 1,2-Dichloroethane-d4	5.034	65	54017	5.775	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	115.400%	
32) Benzene-d6	5.050	84	239335	5.280	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	105.600%	
36) 1,2-Dichloropropane-d6	6.069	67	75643	5.740	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	114.800%	
41) Toluene-d8	7.314	98	193458	4.591	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	91.800%	
43) trans-1,3-Dichloroprop...	7.625	79	18416	4.273	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	85.400%	
46) 2-Hexanone-d5	8.088	63	81309	50.813	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	101.620%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48307	5.691	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	113.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	67988	6.228	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	124.600%#	
Target Compounds						
3) Chloromethane	1.243	50	6901	0.335	ug/L	100
16) Methylene chloride	2.510	84	5036	0.316	ug/L	96
25) Chloroform	4.378	83	8330	0.317	ug/L	94
47) Tetrachloroethene	7.986	164	1338m	0.114	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025941.D
Acq On : 20 May 2022 13:20
Operator : SY/MD
Sample : N2955-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA0

Manual IntegrationsAPPROVED

Quant Time: May 20 21:50:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri May 20 21:49:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/24/2022
Supervised By :Mahesh Dadoda 05/24/2022

