

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025940.D
 Acq On : 20 May 2022 12:51
 Operator : SY/MD
 Sample : VV0520WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK361

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	100	rVB	93259	98763	16.57%	2.024%
2	1.571	157	165	177	rBV	88194	101092	16.96%	2.072%
3	2.111	319	333	348	rVB	178142	262282	44.00%	5.375%
4	2.510	447	457	469	rBV2	15801	27329	4.58%	0.560%
5	3.044	613	623	638	rVB5	5035	10552	1.77%	0.216%
6	3.912	880	893	937	rBV3	44593	177662	29.80%	3.641%
7	4.346	1011	1028	1061	rBV	111717	282052	47.31%	5.780%
8	5.047	1230	1246	1275	rBV2	240050	596138	100.00%	12.217%
9	5.613	1409	1422	1450	rBV	191626	405435	68.01%	8.309%
10	6.066	1545	1563	1591	rBV	141783	295633	49.59%	6.058%
11	6.985	1840	1849	1876	rBV	47149	94400	15.84%	1.935%
12	7.313	1939	1951	1973	rBV	263788	472404	79.24%	9.681%
13	7.625	2039	2048	2066	rBV2	27443	52046	8.73%	1.067%
14	8.088	2182	2192	2237	rBV	191601	428815	71.93%	8.788%
15	8.420	2285	2295	2305	rBV2	13532	22918	3.84%	0.470%
16	8.850	2417	2429	2454	rBV	321879	531522	89.16%	10.892%
17	10.214	2842	2853	2871	rBV	90685	147335	24.71%	3.019%
18	11.246	3164	3174	3193	rBV	307058	482037	80.86%	9.878%
19	11.622	3280	3291	3320	rBV	244334	391327	65.64%	8.019%




Sum of corrected areas: 4879742

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025940.D
Acq On : 20 May 2022 12:51
Operator : SY/MD
Sample : VV0520WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK361

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

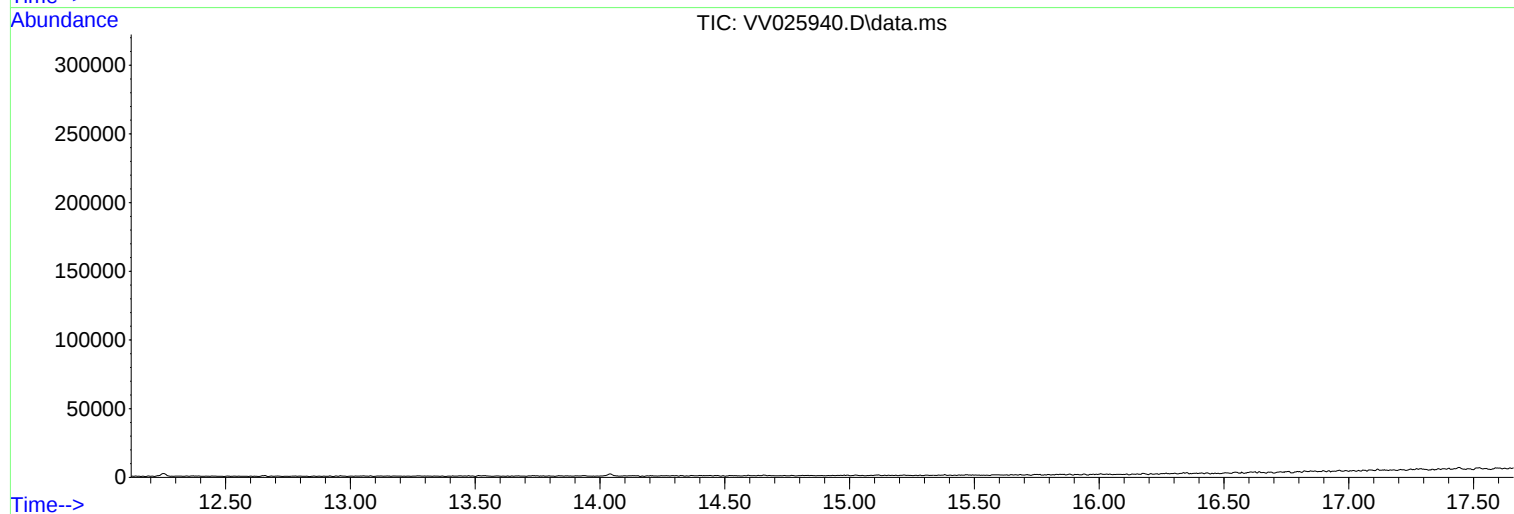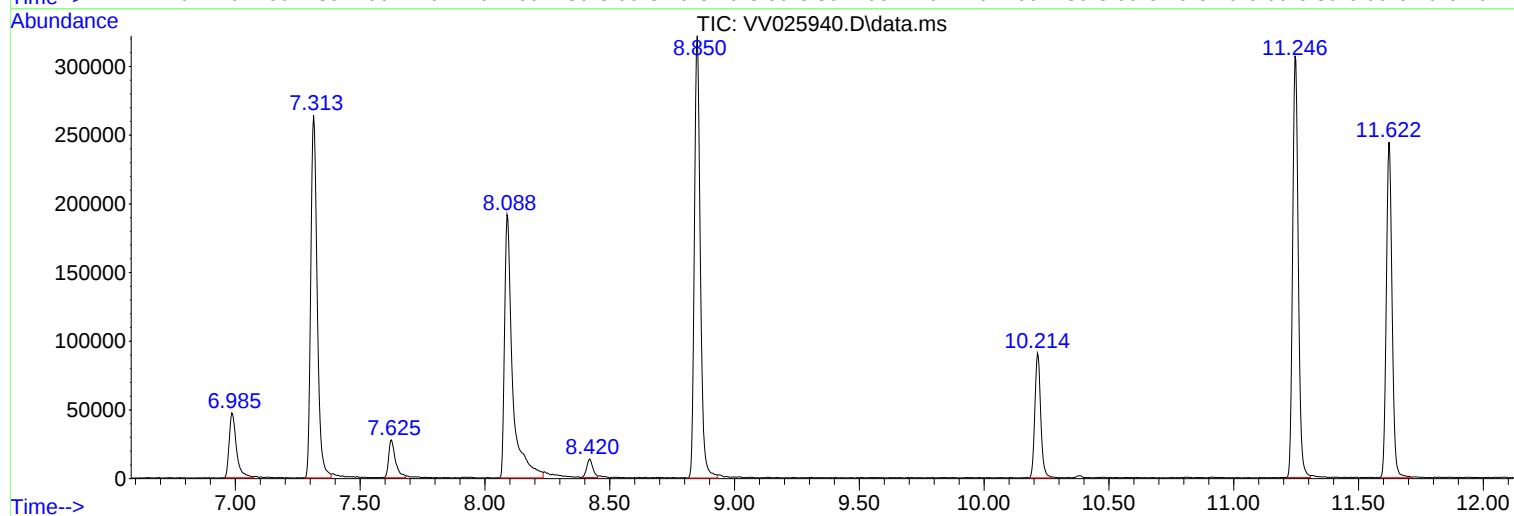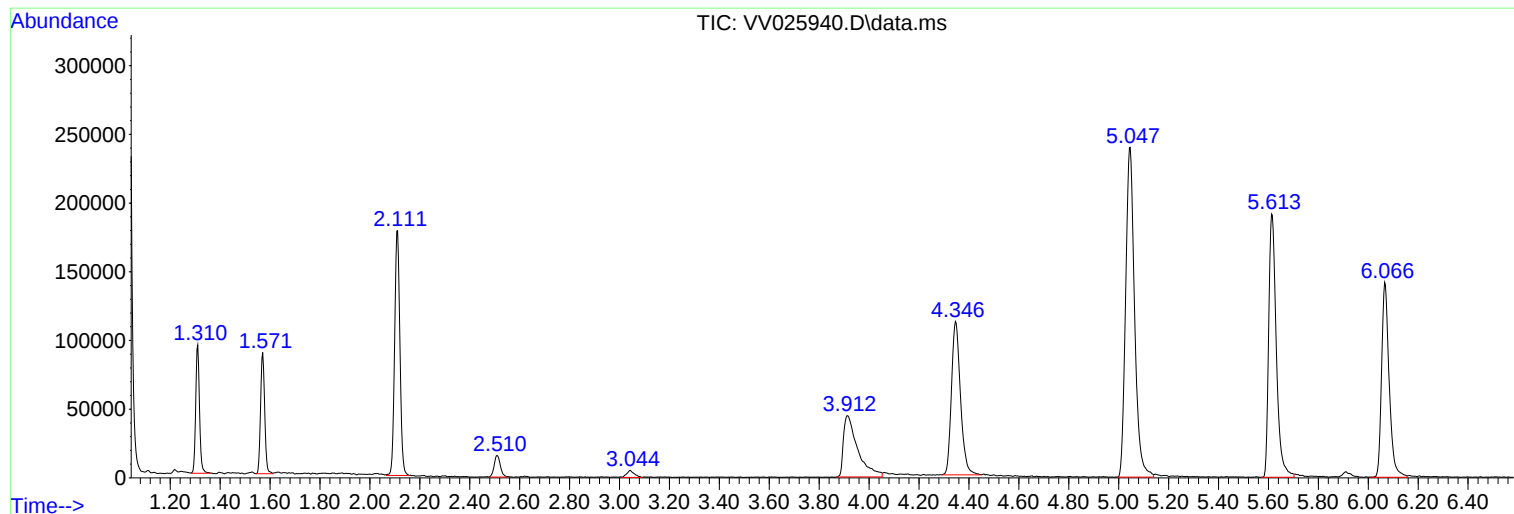

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025940.D
Acq On : 20 May 2022 12:51
Operator : SY/MD
Sample : VV0520WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK361

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025940.D
Acq On : 20 May 2022 12:51
Operator : SY/MD
Sample : VV0520WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK361

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
