

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025942.D
 Acq On : 20 May 2022 13:44
 Operator : SY/MD
 Sample : N2955-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	93573	97589	16.14%	1.998%
2	1.571	157	165	181	rVB	92332	105542	17.46%	2.160%
3	2.111	323	333	351	rVB	182484	268159	44.35%	5.489%
4	3.921	884	896	936	rBV	32906	159459	26.37%	3.264%
5	4.352	1013	1030	1053	rBV	112655	297279	49.17%	6.085%
6	5.050	1229	1247	1274	rBV2	244836	604633	100.00%	12.377%
7	5.619	1412	1424	1451	rBV	177798	368597	60.96%	7.545%
8	5.915	1508	1516	1533	rVB8	3551	8063	1.33%	0.165%
9	6.072	1550	1565	1594	rBV	143021	303653	50.22%	6.216%
10	6.989	1841	1850	1875	rBV	47253	94585	15.64%	1.936%
11	7.317	1937	1952	1974	rBV	263158	476233	78.76%	9.749%
12	7.625	2038	2048	2066	rBV	25643	49746	8.23%	1.018%
13	7.979	2152	2158	2170	rVB6	5374	9996	1.65%	0.205%
14	8.091	2183	2193	2235	rBV	209009	463546	76.67%	9.489%
15	8.255	2235	2244	2252	rBV10	5984	11110	1.84%	0.227%
16	8.854	2418	2430	2461	rBV	295307	489001	80.88%	10.010%
17	10.217	2835	2854	2869	rBV	93773	151288	25.02%	3.097%
18	10.381	2897	2905	2915	rVB3	8339	12745	2.11%	0.261%
19	11.249	3164	3175	3196	rBV	278773	441956	73.09%	9.047%
20	11.529	3253	3262	3276	rBV3	20551	37246	6.16%	0.762%
21	11.622	3280	3291	3310	rVV	254409	406417	67.22%	8.320%
22	12.345	3508	3516	3532	rBV3	9113	14187	2.35%	0.290%
23	12.670	3609	3617	3626	rBV6	5362	7532	1.25%	0.154%
24	15.516	4490	4502	4510	rBV7	4021	6512	1.08%	0.133%


Sum of corrected areas: 4885074

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025942.D
Acq On : 20 May 2022 13:44
Operator : SY/MD
Sample : N2955-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

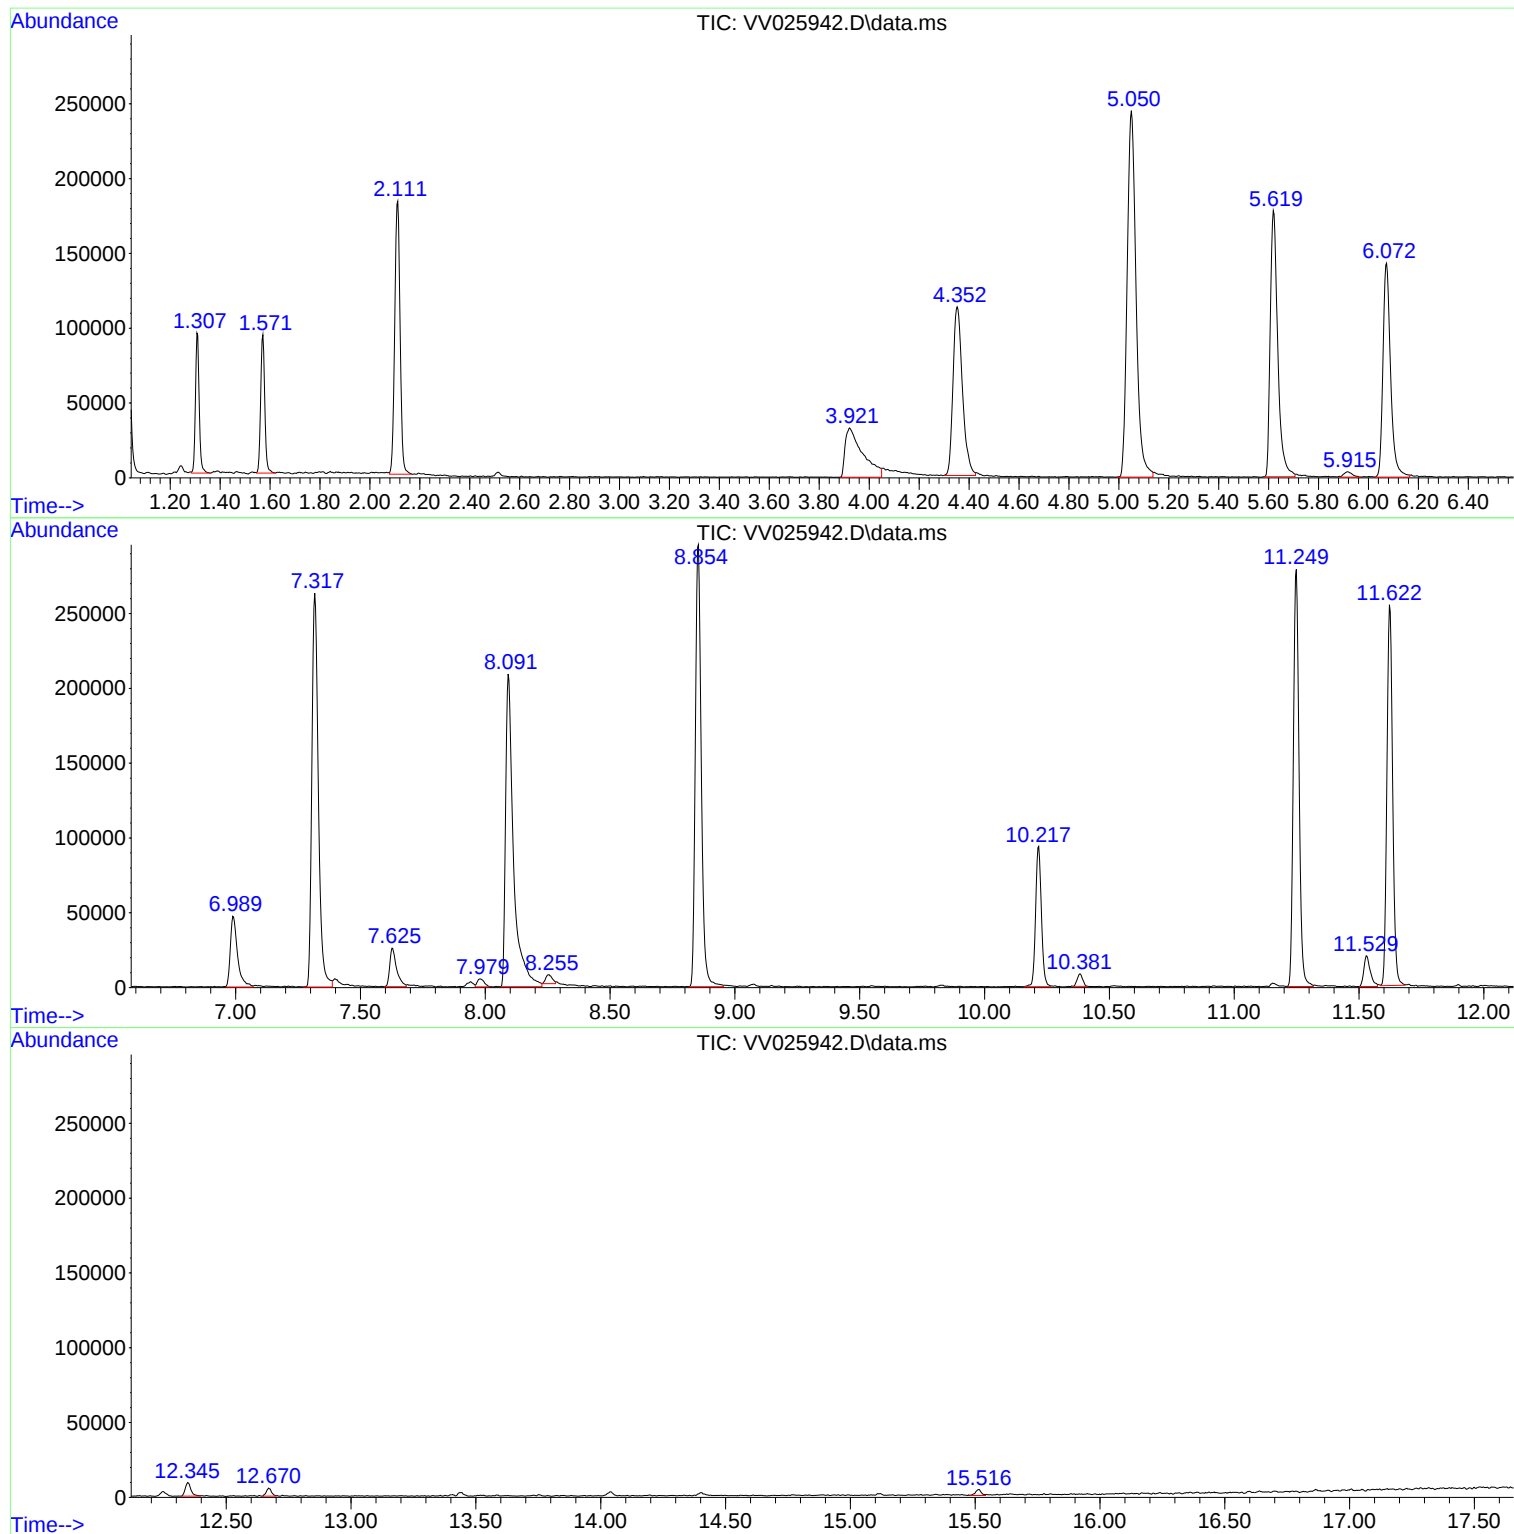

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025942.D
Acq On : 20 May 2022 13:44
Operator : SY/MD
Sample : N2955-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025942.D
Acq On : 20 May 2022 13:44
Operator : SY/MD
Sample : N2955-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc