

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025944.D
 Acq On : 20 May 2022 14:31
 Operator : SY/MD
 Sample : N2955-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	100	rVB	97940	100638	11.76%	1.600%
2	1.571	157	165	178	rBV	92745	104156	12.17%	1.656%
3	2.118	319	335	352	rBV5	450059	753032	88.02%	11.970%
4	3.195	657	670	692	rBV	77052	162771	19.03%	2.587%
5	3.915	884	894	936	rBV	34152	150486	17.59%	2.392%
6	4.352	1015	1030	1058	rBV	114374	286352	33.47%	4.552%
7	4.609	1091	1110	1142	rBV	342846	855521	100.00%	13.599%
8	5.050	1232	1247	1275	rBV3	246321	611336	71.46%	9.718%
9	5.622	1412	1425	1456	rBV	148179	314362	36.75%	4.997%
10	5.918	1504	1517	1541	rBV	126417	260898	30.50%	4.147%
11	6.072	1551	1565	1595	rBV	143113	301649	35.26%	4.795%
12	6.992	1839	1851	1879	rBV	49783	100712	11.77%	1.601%
13	7.317	1941	1952	1975	rBV	268735	478589	55.94%	7.607%
14	7.629	2038	2049	2066	rBV2	26516	51982	6.08%	0.826%
15	8.092	2184	2193	2232	rBV	185302	442807	51.76%	7.039%
16	8.854	2416	2430	2461	rBV	240258	408286	47.72%	6.490%
17	10.217	2841	2854	2869	rBV	92430	149789	17.51%	2.381%
18	10.381	2895	2905	2919	rVB4	6574	9591	1.12%	0.152%
19	11.249	3164	3175	3191	rBV	227549	351262	41.06%	5.584%
20	11.535	3256	3264	3276	rBV5	5296	9702	1.13%	0.154%
21	11.622	3279	3291	3310	rBV	245809	387113	45.25%	6.153%




Sum of corrected areas: 6291034

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025944.D
Acq On : 20 May 2022 14:31
Operator : SY/MD
Sample : N2955-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

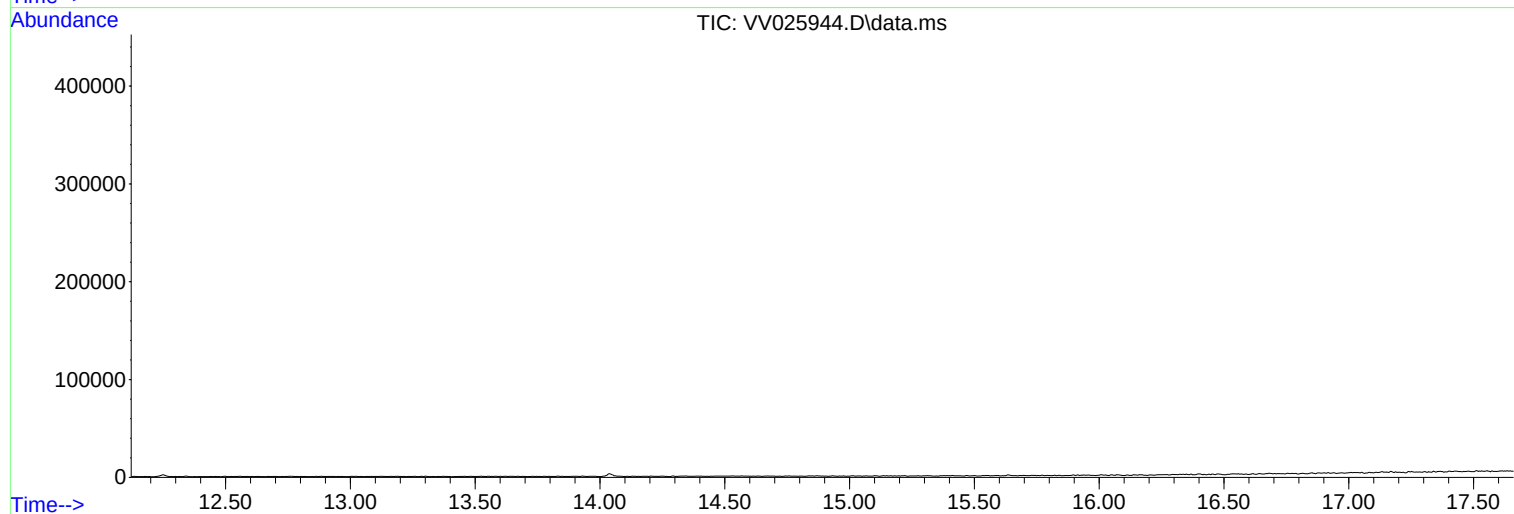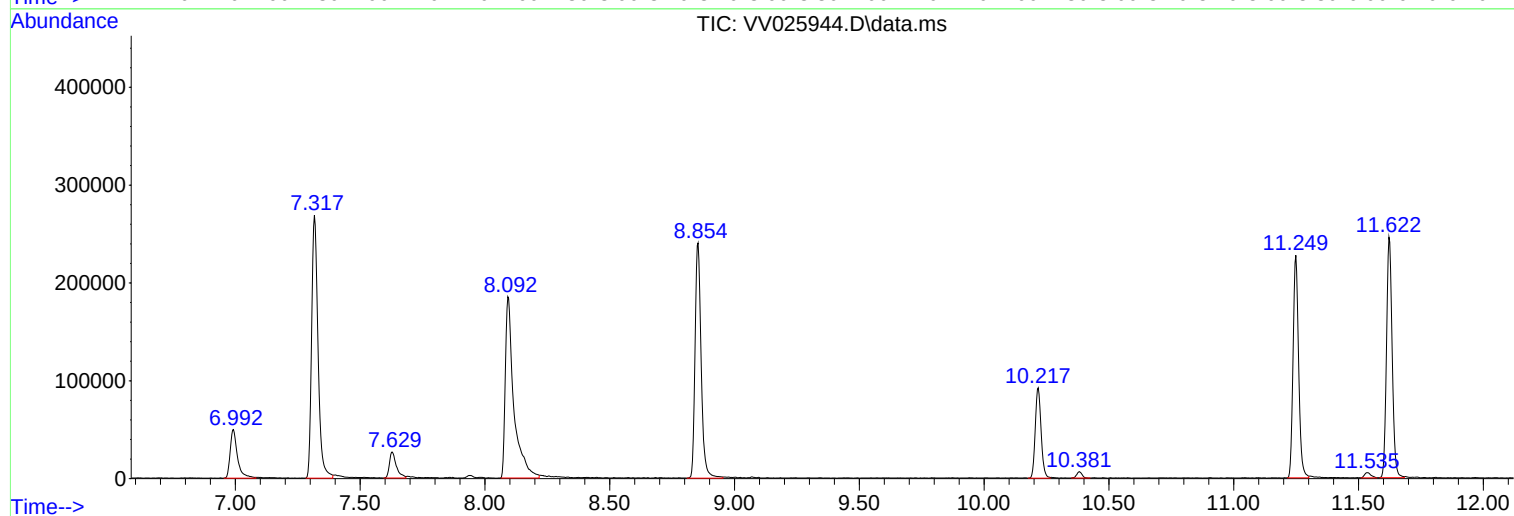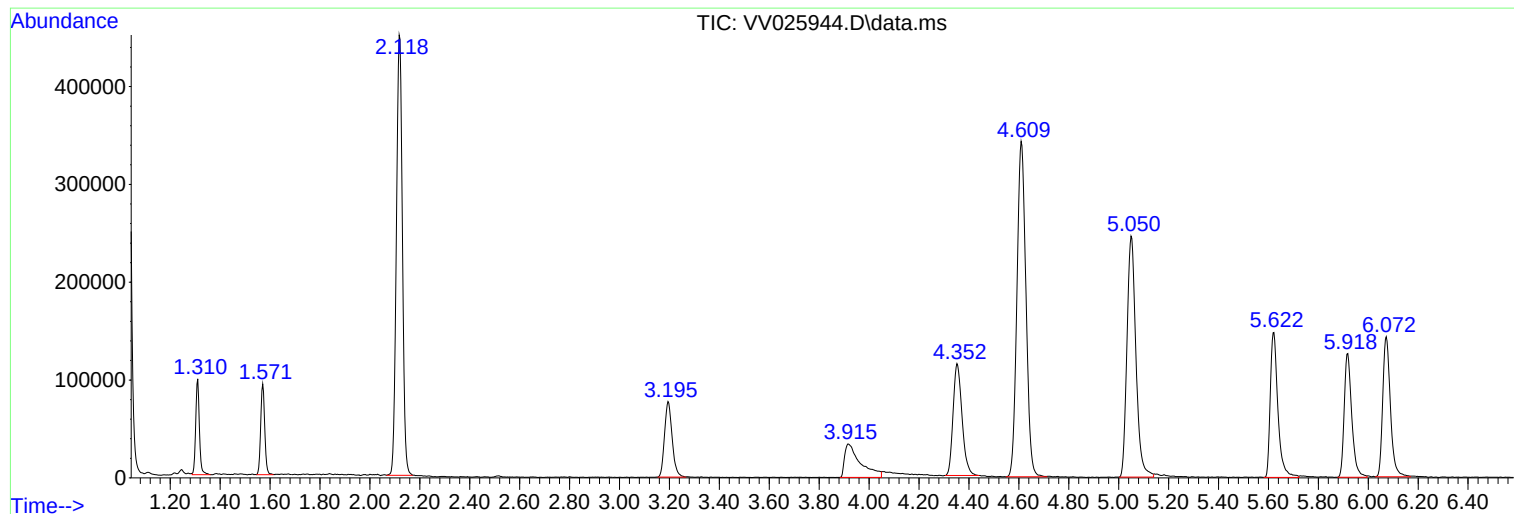

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025944.D
Acq On : 20 May 2022 14:31
Operator : SY/MD
Sample : N2955-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025944.D
Acq On : 20 May 2022 14:31
Operator : SY/MD
Sample : N2955-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc