

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025945.D
 Acq On : 20 May 2022 14:54
 Operator : SY/MD
 Sample : N2955-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	93	rBV	86077	87900	10.39%	1.436%
2	1.571	158	165	181	rBV	86595	100054	11.83%	1.635%
3	2.121	322	336	361	rVB4	433661	717345	84.80%	11.722%
4	3.195	655	670	693	rBV2	75559	163014	19.27%	2.664%
5	3.908	879	892	910	rBV2	30850	102725	12.14%	1.679%
6	4.352	1013	1030	1061	rVB	108437	280013	33.10%	4.575%
7	4.609	1091	1110	1134	rBV2	338395	845918	100.00%	13.822%
8	5.053	1232	1248	1273	rBV2	229504	571996	67.62%	9.346%
9	5.619	1413	1424	1448	rBV	162420	342863	40.53%	5.602%
10	5.918	1504	1517	1538	rBV	126434	259445	30.67%	4.239%
11	6.072	1553	1565	1594	rBV	133653	282331	33.38%	4.613%
12	6.992	1838	1851	1871	rBV2	48162	91869	10.86%	1.501%
13	7.317	1940	1952	1974	rBV	255304	445955	52.72%	7.287%
14	7.628	2040	2049	2067	rBV2	25585	47846	5.66%	0.782%
15	8.091	2179	2193	2236	rBV	160550	417403	49.34%	6.820%
16	8.853	2419	2430	2456	rBV	271062	449946	53.19%	7.352%
17	10.217	2841	2854	2868	rBV	86171	141969	16.78%	2.320%
18	10.381	2897	2905	2918	rVB4	6625	11129	1.32%	0.182%
19	11.249	3163	3175	3198	rBV	254522	394480	46.63%	6.446%
20	11.622	3281	3291	3313	rBV	227464	365702	43.23%	5.976%




Sum of corrected areas: 6119903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025945.D
Acq On : 20 May 2022 14:54
Operator : SY/MD
Sample : N2955-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

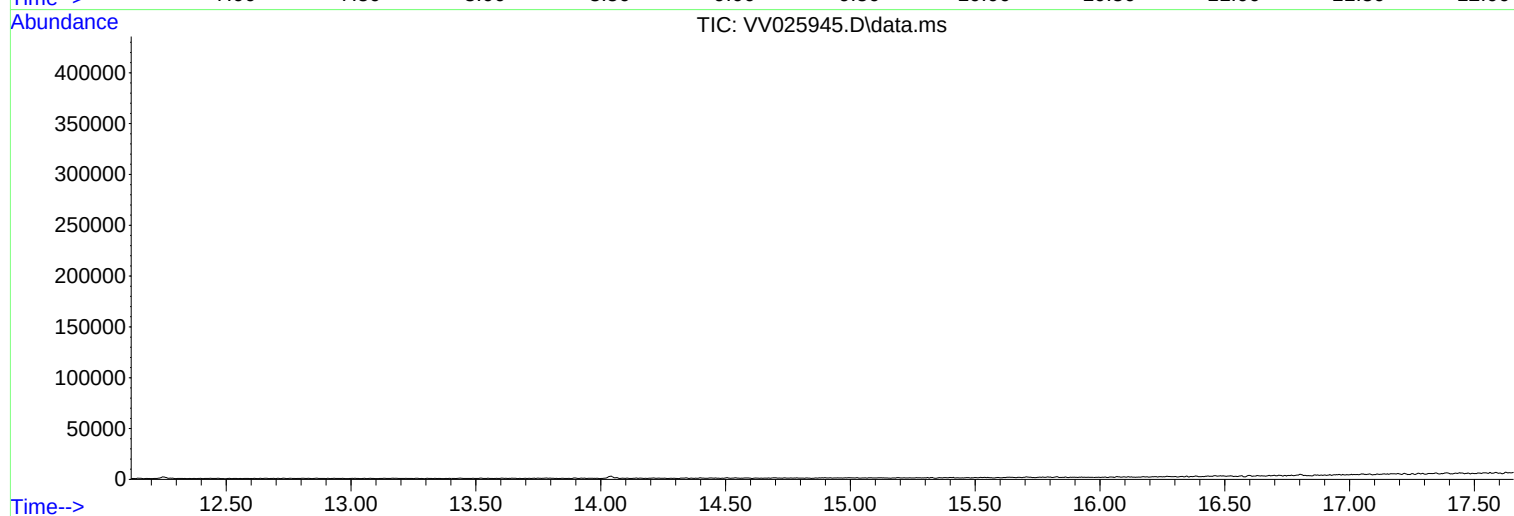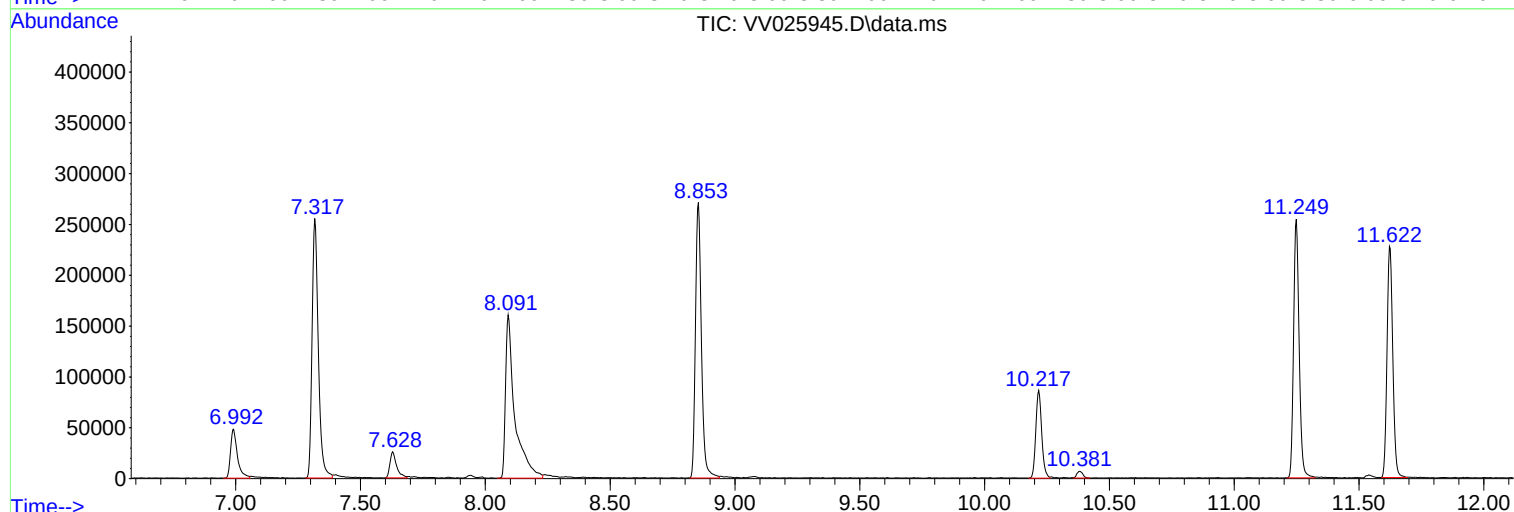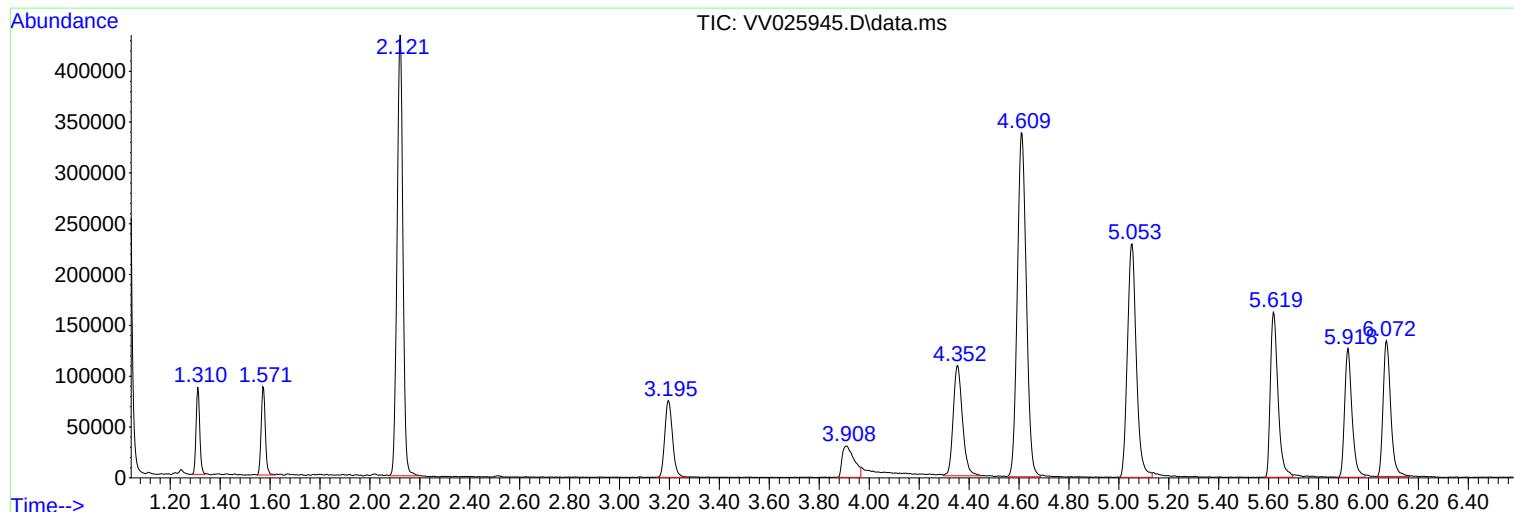

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025945.D
Acq On : 20 May 2022 14:54
Operator : SY/MD
Sample : N2955-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025945.D
Acq On : 20 May 2022 14:54
Operator : SY/MD
Sample : N2955-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc