

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025946.D
 Acq On : 20 May 2022 15:18
 Operator : SY/MD
 Sample : N2955-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	96	rVB	80404	82706	9.80%	1.408%
2	1.571	157	165	176	rBV	81424	91175	10.81%	1.552%
3	2.121	322	336	354	rBV4	427022	696344	82.55%	11.854%
4	3.194	653	670	688	rBV	76104	161868	19.19%	2.755%
5	3.908	883	892	894	rBV	24899	30177	3.58%	0.514%
6	4.352	1014	1030	1061	rVB	98089	251758	29.84%	4.286%
7	4.609	1091	1110	1137	rBV	335737	843590	100.00%	14.361%
8	5.050	1230	1247	1272	rBV3	206784	517432	61.34%	8.808%
9	5.619	1413	1424	1450	rBV	171910	354109	41.98%	6.028%
10	5.918	1503	1517	1539	rBV	126469	261382	30.98%	4.450%
11	6.072	1551	1565	1586	rBV2	123340	260299	30.86%	4.431%
12	6.992	1840	1851	1876	rBV	40860	83631	9.91%	1.424%
13	7.317	1942	1952	1977	rBV	228293	410317	48.64%	6.985%
14	7.628	2036	2049	2072	rBV2	22535	44579	5.28%	0.759%
15	8.091	2183	2193	2228	rBV	142289	380390	45.09%	6.475%
16	8.853	2419	2430	2459	rBV	281295	469929	55.71%	8.000%
17	10.217	2843	2854	2870	rBV	80834	131307	15.57%	2.235%
18	10.381	2896	2905	2914	rVB3	6994	11156	1.32%	0.190%
19	11.249	3164	3175	3191	rBV	265576	414349	49.12%	7.054%
20	11.532	3254	3263	3280	rBV2	17665	32220	3.82%	0.548%
21	11.625	3280	3292	3310	rVB	213644	345647	40.97%	5.884%




Sum of corrected areas: 5874365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025946.D
Acq On : 20 May 2022 15:18
Operator : SY/MD
Sample : N2955-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

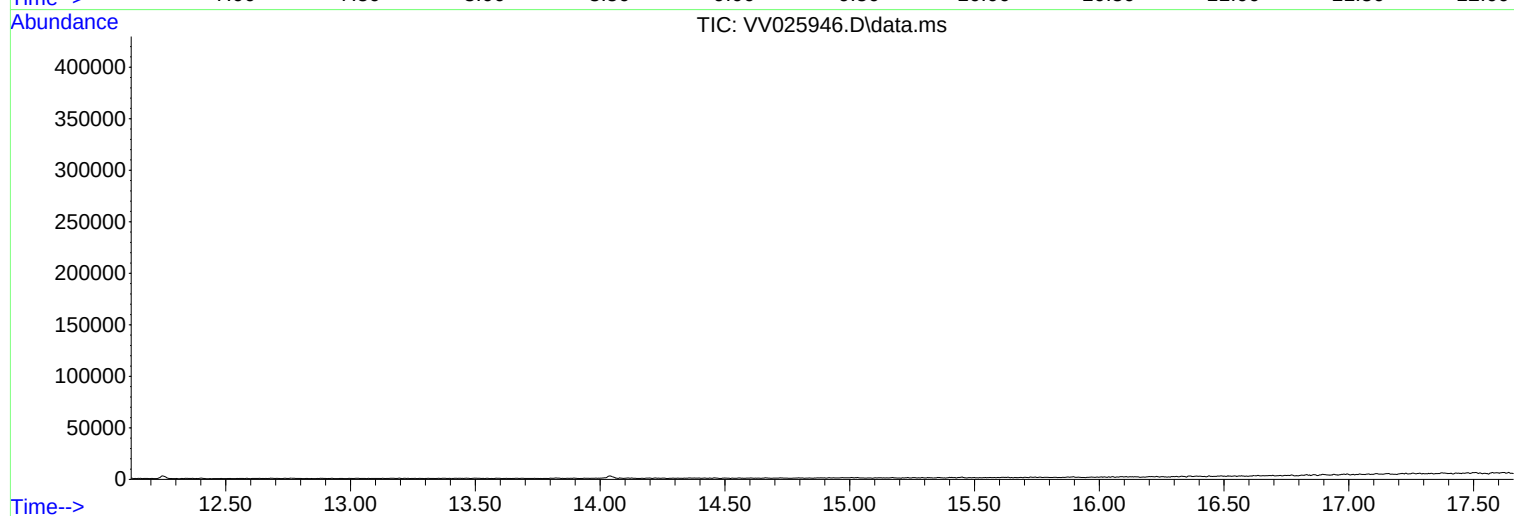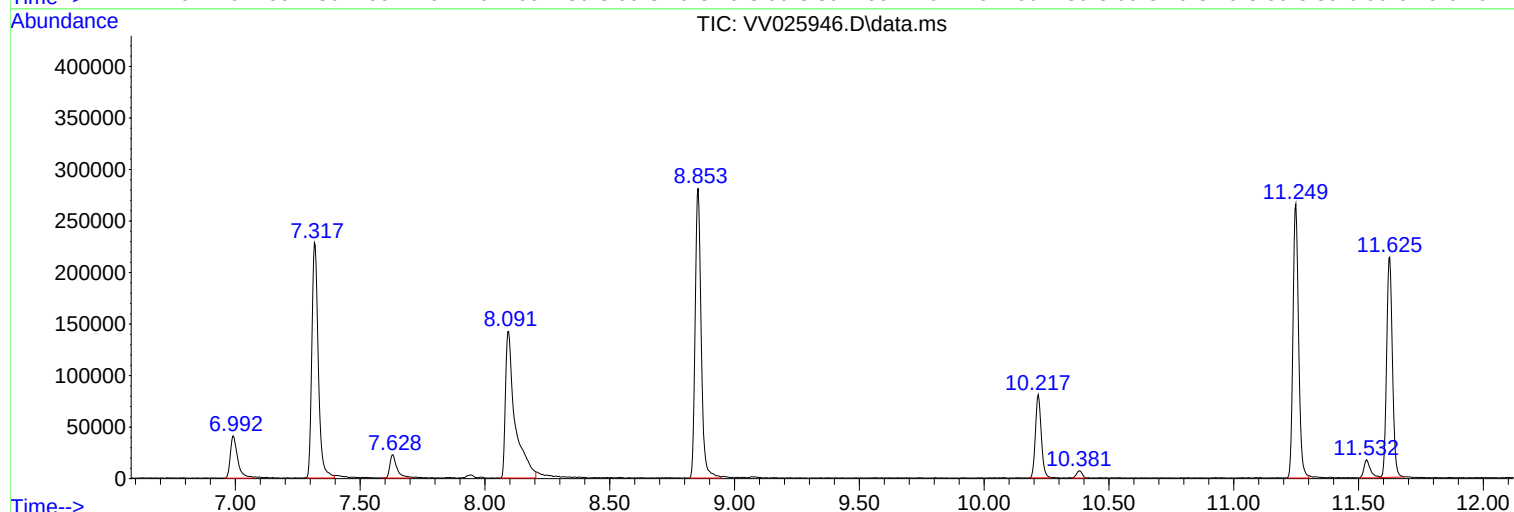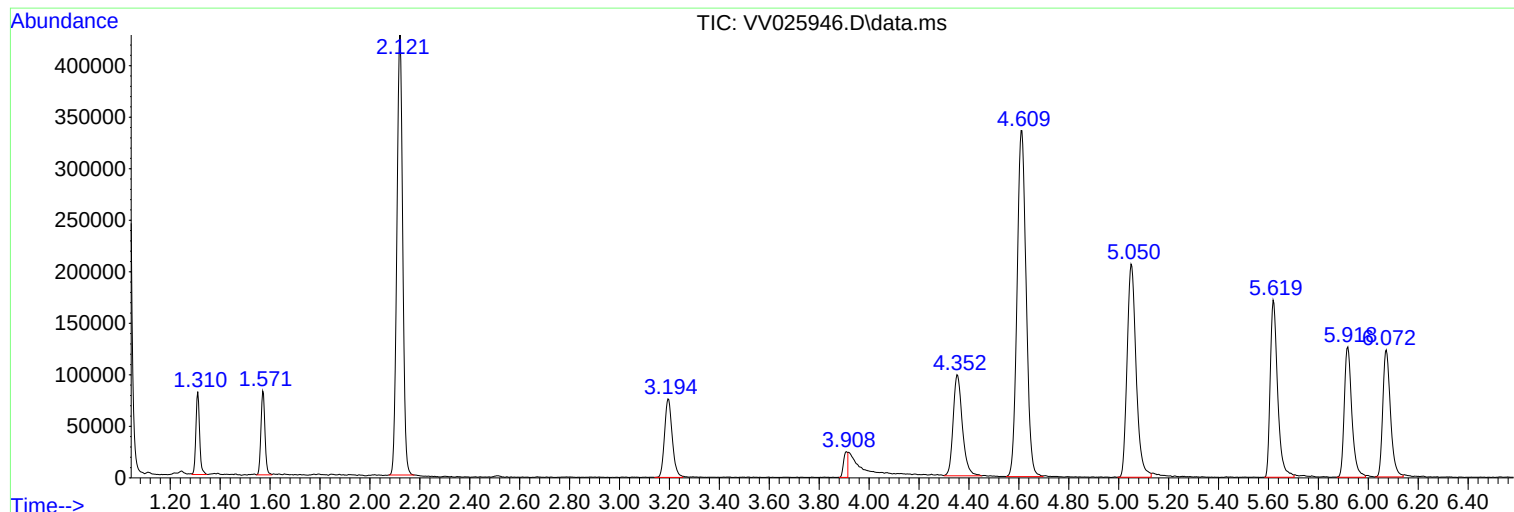

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025946.D
Acq On : 20 May 2022 15:18
Operator : SY/MD
Sample : N2955-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
Data File : VV025946.D
Acq On : 20 May 2022 15:18
Operator : SY/MD
Sample : N2955-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc