
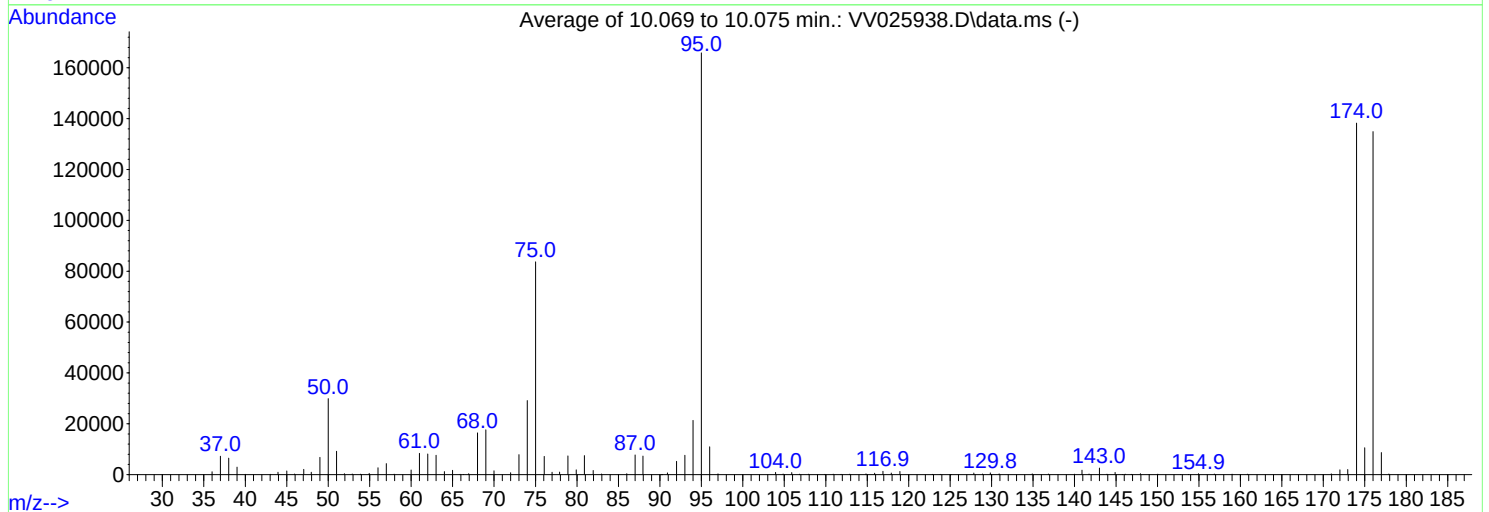


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052022\
 Data File : VV025938.D
 Acq On : 20 May 2022 08:53
 Operator : SY/MD
 Sample : BFB319
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB319

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue May 24 05:29:18 2022

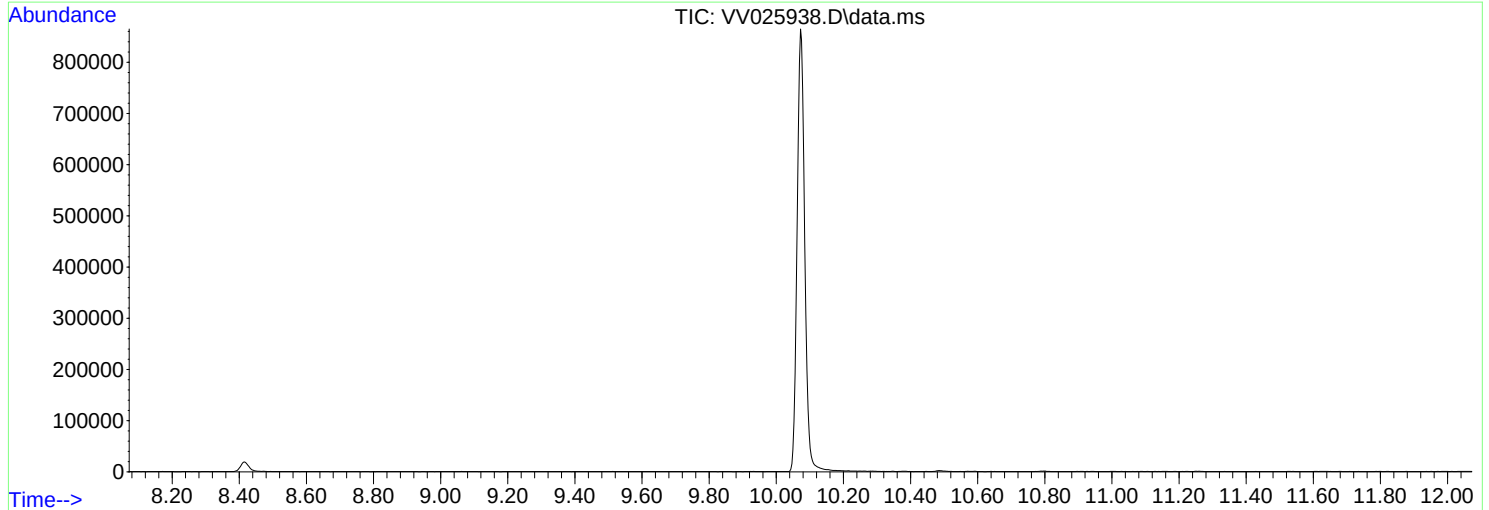

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	29875	PASS
75	95	30	80	50.5	83709	PASS
95	95	100	100	100.0	165867	PASS
96	95	5	9	6.6	10928	PASS
173	174	0.00	2	1.4	2001	PASS
174	95	50	120	83.3	138208	PASS
175	174	5	9	7.7	10577	PASS
176	174	95	105	97.6	134880	PASS
177	176	5	10	6.4	8681	PASS

m/z	Abundance
40.00	206.0
40.80	131.0
43.90	363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB319

m/z	Abundance
36.00	1259.0
37.00	7110.0
38.00	6164.0
39.00	3082.0
40.10	303.0
43.10	167.0
44.00	1300.0
45.00	1383.0
45.90	275.0
47.10	2106.0
48.00	870.0
49.00	6765.0
50.00	29024.0
51.00	8791.0
52.00	427.0
52.90	192.0
53.90	195.0
55.00	437.0
56.00	2709.0
57.00	4259.0
57.90	252.0
60.00	1795.0
61.00	8026.0
62.00	8024.0
63.00	7411.0
64.00	1268.0
65.00	1571.0
66.30	212.0
67.00	428.0
68.00	15769.0
69.00	16880.0
70.00	1421.0
72.00	720.0
73.00	7672.0
74.00	27880.0
75.00	80360.0
76.00	7228.0
77.00	1016.0
77.90	904.0
78.90	7314.0
79.90	1851.0
80.90	7107.0
82.00	1586.0
83.00	231.0
86.00	409.0
87.00	7556.0
87.90	7078.0
90.90	713.0
92.00	5027.0
93.00	7542.0
94.00	20352.0
95.00	159296.0
96.00	10803.0
97.00	292.0
104.00	850.0
104.80	226.0
105.90	711.0
107.00	170.0
108.00	160.0
109.90	110.0
110.90	157.0
111.80	142.0
112.90	174.0
114.90	255.0
115.90	510.0
116.90	1243.0
117.90	632.0
118.90	1288.0
122.90	119.0
123.80	136.0
127.90	651.0
128.90	242.0
129.90	595.0
131.00	312.0
134.80	363.0
136.80	281.0
140.00	167.0
140.90	1583.0
141.80	235.0
143.00	2552.0
143.90	155.0
144.90	976.0
145.80	229.0
146.80	130.0
148.00	378.0
149.00	130.0
150.10	146.0
153.80	109.0
155.00	305.0
156.90	248.0
159.10	201.0
160.80	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB319

170.90	325.0
172.00	1717.0
173.00	1922.0
174.00	129504.0
175.00	9910.0
176.00	126560.0
177.00	8293.0
177.90	302.0

Instrument :
MSVOA_V
ClientSampleId :
BFB319

m/z	Abundance
36.00	1197.0
37.00	7443.0
38.00	6656.0
39.00	3023.0
40.10	315.0
43.10	148.0
44.00	1314.0
45.00	1535.0
45.90	265.0
47.00	2253.0
48.00	993.0
49.00	7026.0
50.00	30872.0
51.00	9479.0
52.00	392.0
52.90	265.0
53.90	216.0
55.00	517.0
56.00	2820.0
57.00	4520.0
58.00	209.0
60.00	1935.0
61.00	8689.0
62.00	8358.0
63.00	7948.0
64.00	1221.0
65.00	1732.0
65.90	234.0
66.90	400.0
68.00	17032.0
69.00	18360.0
70.00	1590.0
72.00	790.0
73.00	8109.0
74.00	30072.0
75.00	86680.0
76.00	7385.0
77.00	944.0
77.90	1042.0
78.90	7654.0
79.90	1966.0
80.90	7768.0
81.90	1679.0
83.00	258.0
86.00	400.0
87.00	8030.0
88.00	7559.0
90.90	738.0
92.00	5335.0
93.00	7807.0
94.00	22048.0
95.00	171584.0
96.00	11353.0
97.00	305.0
103.90	921.0
104.90	278.0
105.90	876.0
106.80	174.0
107.90	189.0
109.90	130.0
110.90	193.0
111.80	156.0
112.90	174.0
114.80	300.0
115.90	597.0
116.90	1374.0
117.90	654.0
118.90	1315.0
122.90	133.0
123.80	150.0
127.90	649.0
128.90	277.0
129.90	717.0
130.90	325.0
134.90	343.0
136.90	282.0
140.00	196.0
140.90	1812.0
141.70	260.0
143.00	2701.0
143.90	210.0
144.90	924.0
146.10	273.0
146.80	147.0
148.00	384.0
149.00	118.0
150.00	200.0
154.90	404.0
156.80	278.0
159.00	191.0
160.80	185.0
170.90	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB319

172.00	1981.0
173.00	2095.0
174.00	143168.0
175.00	10913.0
176.00	140032.0
177.00	9008.0
177.90	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB319

m/z	Abundance
36.00	1016.0
37.00	7199.0
38.00	6627.0
39.00	2759.0
40.00	334.0
43.00	136.0
44.00	1273.0
45.00	1523.0
46.00	266.0
47.00	1951.0
47.90	1068.0
49.00	6693.0
50.00	29728.0
51.00	9264.0
51.90	359.0
52.90	301.0
53.90	192.0
54.90	587.0
56.00	2615.0
57.00	4268.0
58.00	155.0
60.00	1808.0
61.00	8466.0
62.00	8043.0
63.00	7550.0
64.00	1062.0
65.00	1797.0
65.90	237.0
66.90	414.0
68.00	16504.0
69.00	17688.0
70.00	1560.0
72.00	830.0
73.00	7916.0
74.00	29376.0
75.00	84088.0
76.10	6895.0
77.00	879.0
77.90	1016.0
78.90	7160.0
79.90	1893.0
80.90	7550.0
81.90	1622.0
82.90	207.0
86.00	310.0
87.00	7643.0
88.00	7363.0
90.20	111.0
90.90	709.0
92.00	5299.0
93.00	7539.0
94.00	21512.0
95.00	166720.0
96.00	10629.0
97.00	297.0
103.90	837.0
104.90	319.0
105.90	888.0
106.70	174.0
107.90	175.0
109.90	149.0
110.90	218.0
111.90	167.0
112.90	182.0
114.80	313.0
115.90	605.0
116.90	1339.0
117.90	693.0
119.00	1238.0
122.80	121.0
123.80	131.0
125.00	106.0
127.80	582.0
128.90	278.0
129.80	748.0
130.80	265.0
135.00	344.0
136.90	272.0
140.00	174.0
140.90	1856.0
141.70	260.0
143.00	2538.0
143.90	212.0
144.90	778.0
146.10	354.0
146.90	163.0
147.90	428.0
150.00	253.0
152.80	137.0
153.70	111.0
154.90	460.0
156.80	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB319

158.90	192.0
160.90	159.0
171.00	286.0
172.00	2041.0
172.90	1985.0
174.00	141952.0
175.00	10908.0
176.00	138048.0
177.00	8741.0
177.90	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB319