
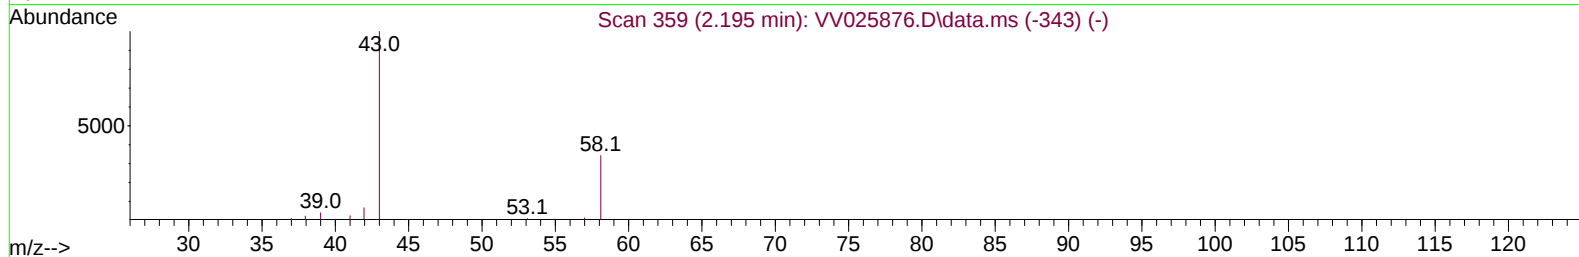
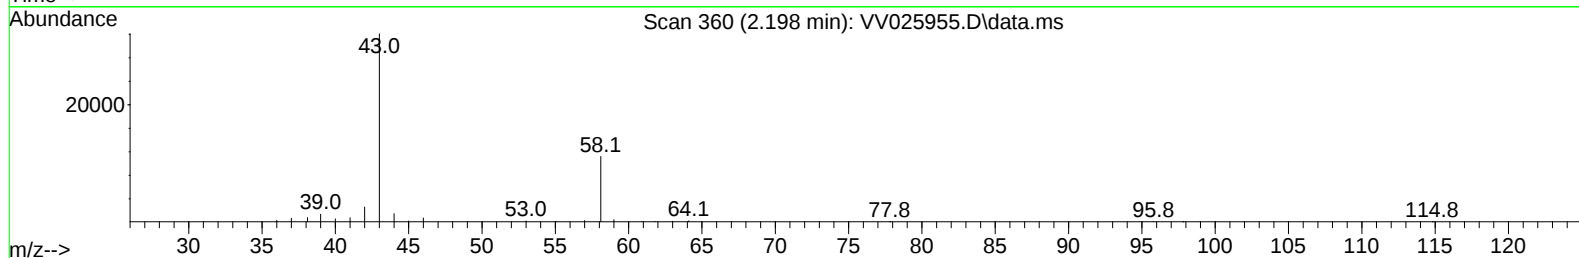


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052622\
Data File : VW025955.D
Acq On : 26 May 2022 12:39
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 27 01:21:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 07:07:32 2022
Response via : Initial Calibration

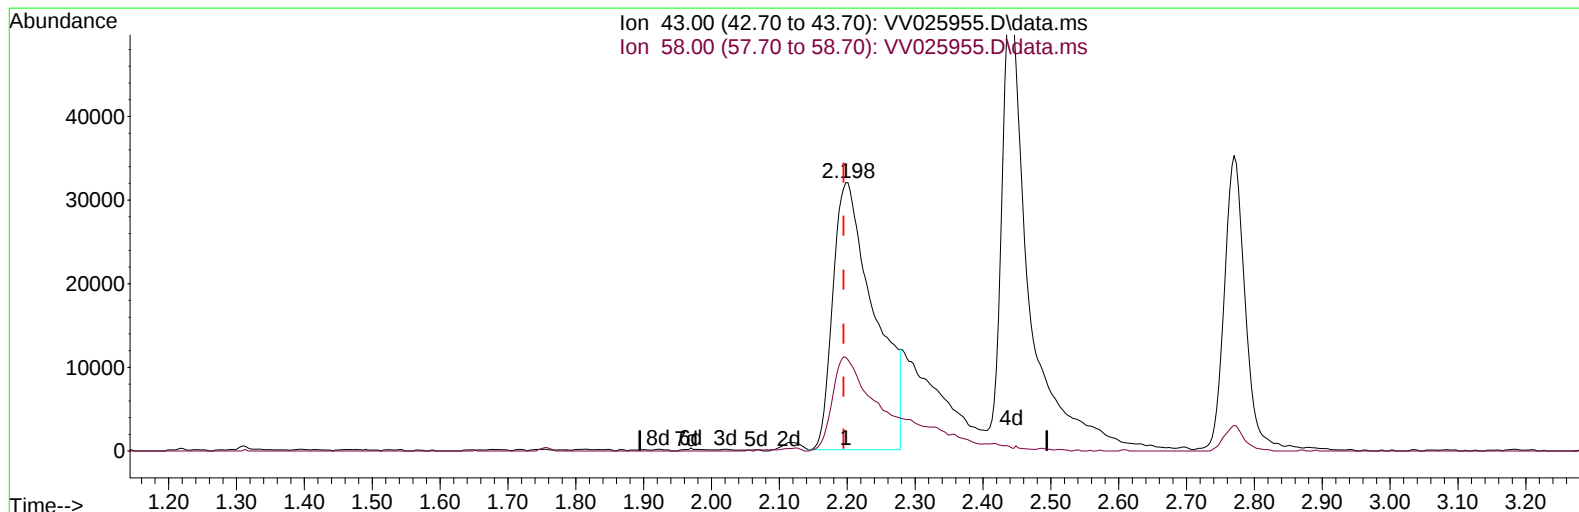

TIC: VV025955.D\data.ms

(13) Acetone (T)

2.198min (+ 0.003) 91.94 ug/L

response **134948**

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	36.79
0.00	0.00	0.00
0.00	0.00	0.00