

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025956.D
 Acq On : 26 May 2022 14:20
 Operator : SY/MD
 Sample : VV0526WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Quant Time: May 27 01:28:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 01:28:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	351541	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	343294	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	158868	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	194421	42.853	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.700%		
7) Chloroethane-d5	1.571	69	155429	39.011	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.020%		
11) 1,1-Dichloroethene-d2	2.108	63	272412	34.330	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.660%		
21) 2-Butanone-d5	3.899	46	152219	78.278	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	78.280%		
24) Chloroform-d	4.346	84	275720	43.510	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.020%		
26) 1,2-Dichloroethane-d4	5.027	65	171056	44.664	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.320%		
32) Benzene-d6	5.047	84	565309	47.236	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.480%		
36) 1,2-Dichloropropane-d6	6.066	67	177651	48.330	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.660%		
41) Toluene-d8	7.313	98	485723	44.050	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.100%		
43) trans-1,3-Dichloroprop...	7.619	79	66722	40.664	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.320%		
47) 2-Hexanone-d5	8.088	63	101732	75.490	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	75.490%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	216599	44.187	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.380%		
66) 1,2-Dichlorobenzene-d4	11.622	152	174592	50.100	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.200%		
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.104	101	2687	0.796	ug/L #	22
61) 1,2,3-Trichloropropane	11.246	75	19052	6.059	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025956.D
Acq On : 26 May 2022 14:20
Operator : SY/MD
Sample : VV0526WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Time: May 27 01:28:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 27 01:28:09 2022
Response via : Initial Calibration




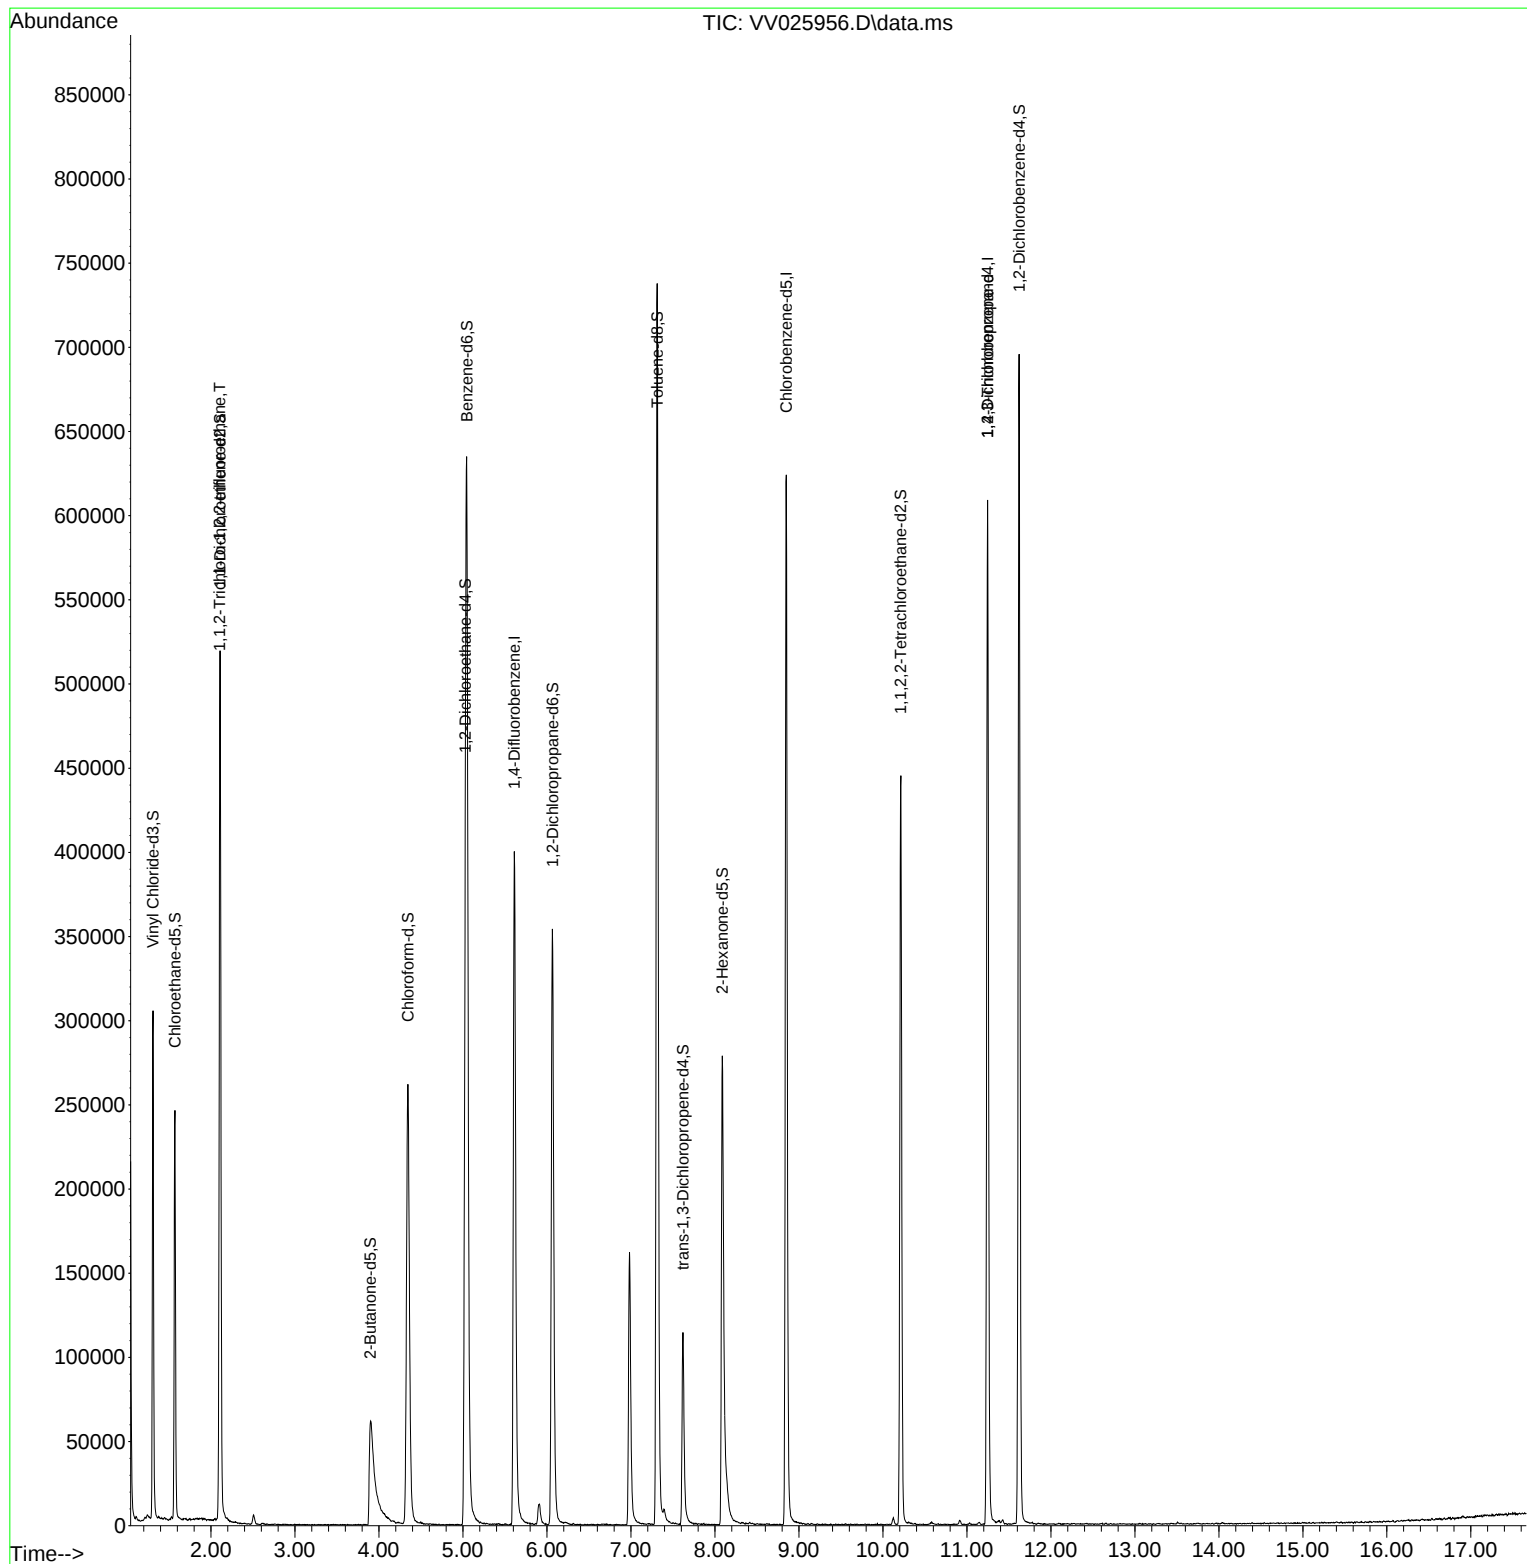


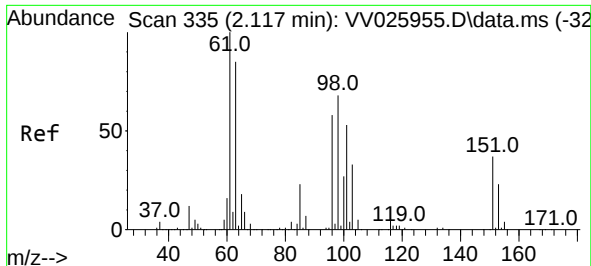

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.796 ug/L
 RT: 2.104 min Scan# 31
 Delta R.T. -0.013 min
 Lab File: VV025956.D
 Acq: 26 May 2022 14:20

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Tgt Ion:101 Resp: 2687
 Ion Ratio Lower Upper
 101 100
 85 0.0 34.6 51.8#
 151 0.0 54.3 81.5#

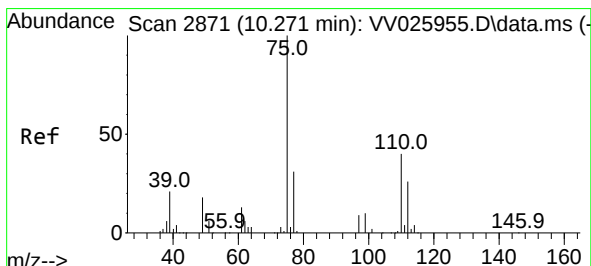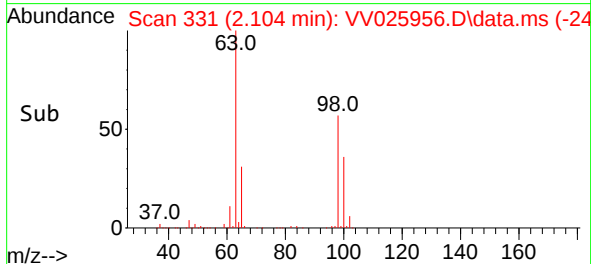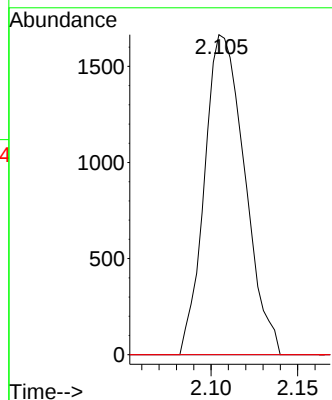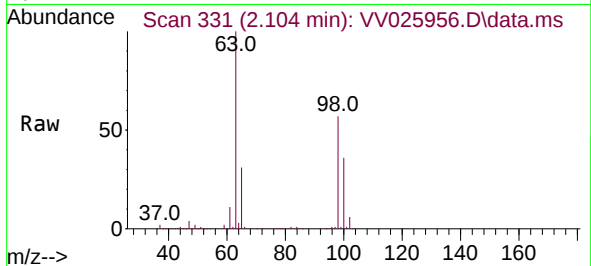

#61
 1,2,3-Trichloropropane
 Concen: 6.059 ug/L
 RT: 11.246 min Scan# 3174
 Delta R.T. 0.974 min
 Lab File: VV025956.D
 Acq: 26 May 2022 14:20

Tgt Ion: 75 Resp: 19052
 Ion Ratio Lower Upper
 75 100
 77 32.7 25.3 37.9
 110 3.1 32.3 48.5#

