

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052622\
 Data File : VW025957.D
 Acq On : 26 May 2022 14:48
 Operator : SY/MD
 Sample : N3039-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JR7

Quant Time: May 27 01:29:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 01:28:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	345041	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	347382	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	156764	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	181104	40.669	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.340%
7) Chloroethane-d5	1.571	69	147067	37.607	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	75.220%
11) 1,1-Dichloroethene-d2	2.108	63	257469	33.059	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.120%
21) 2-Butanone-d5	3.905	46	123536	64.725	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	64.720%
24) Chloroform-d	4.346	84	260893	41.946	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.900%
26) 1,2-Dichloroethane-d4	5.031	65	160753	42.764	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.520%
32) Benzene-d6	5.047	84	534508	44.137	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.280%
36) 1,2-Dichloropropane-d6	6.066	67	167378	45.000	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.000%
41) Toluene-d8	7.313	98	460360	41.258	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.520%
43) trans-1,3-Dichloroprop...	7.622	79	62893	37.879	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.760%
47) 2-Hexanone-d5	8.088	63	92698	67.977	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.980%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	202745	40.874	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	81.740%
66) 1,2-Dichlorobenzene-d4	11.622	152	166213	48.336	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.680%
Target Compounds						
61) 1,2,3-Trichloropropane	11.246	75	19133	6.166	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025957.D
Acq On : 26 May 2022 14:48
Operator : SY/MD
Sample : N3039-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JR7

Quant Time: May 27 01:29:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 27 01:28:09 2022
Response via : Initial Calibration

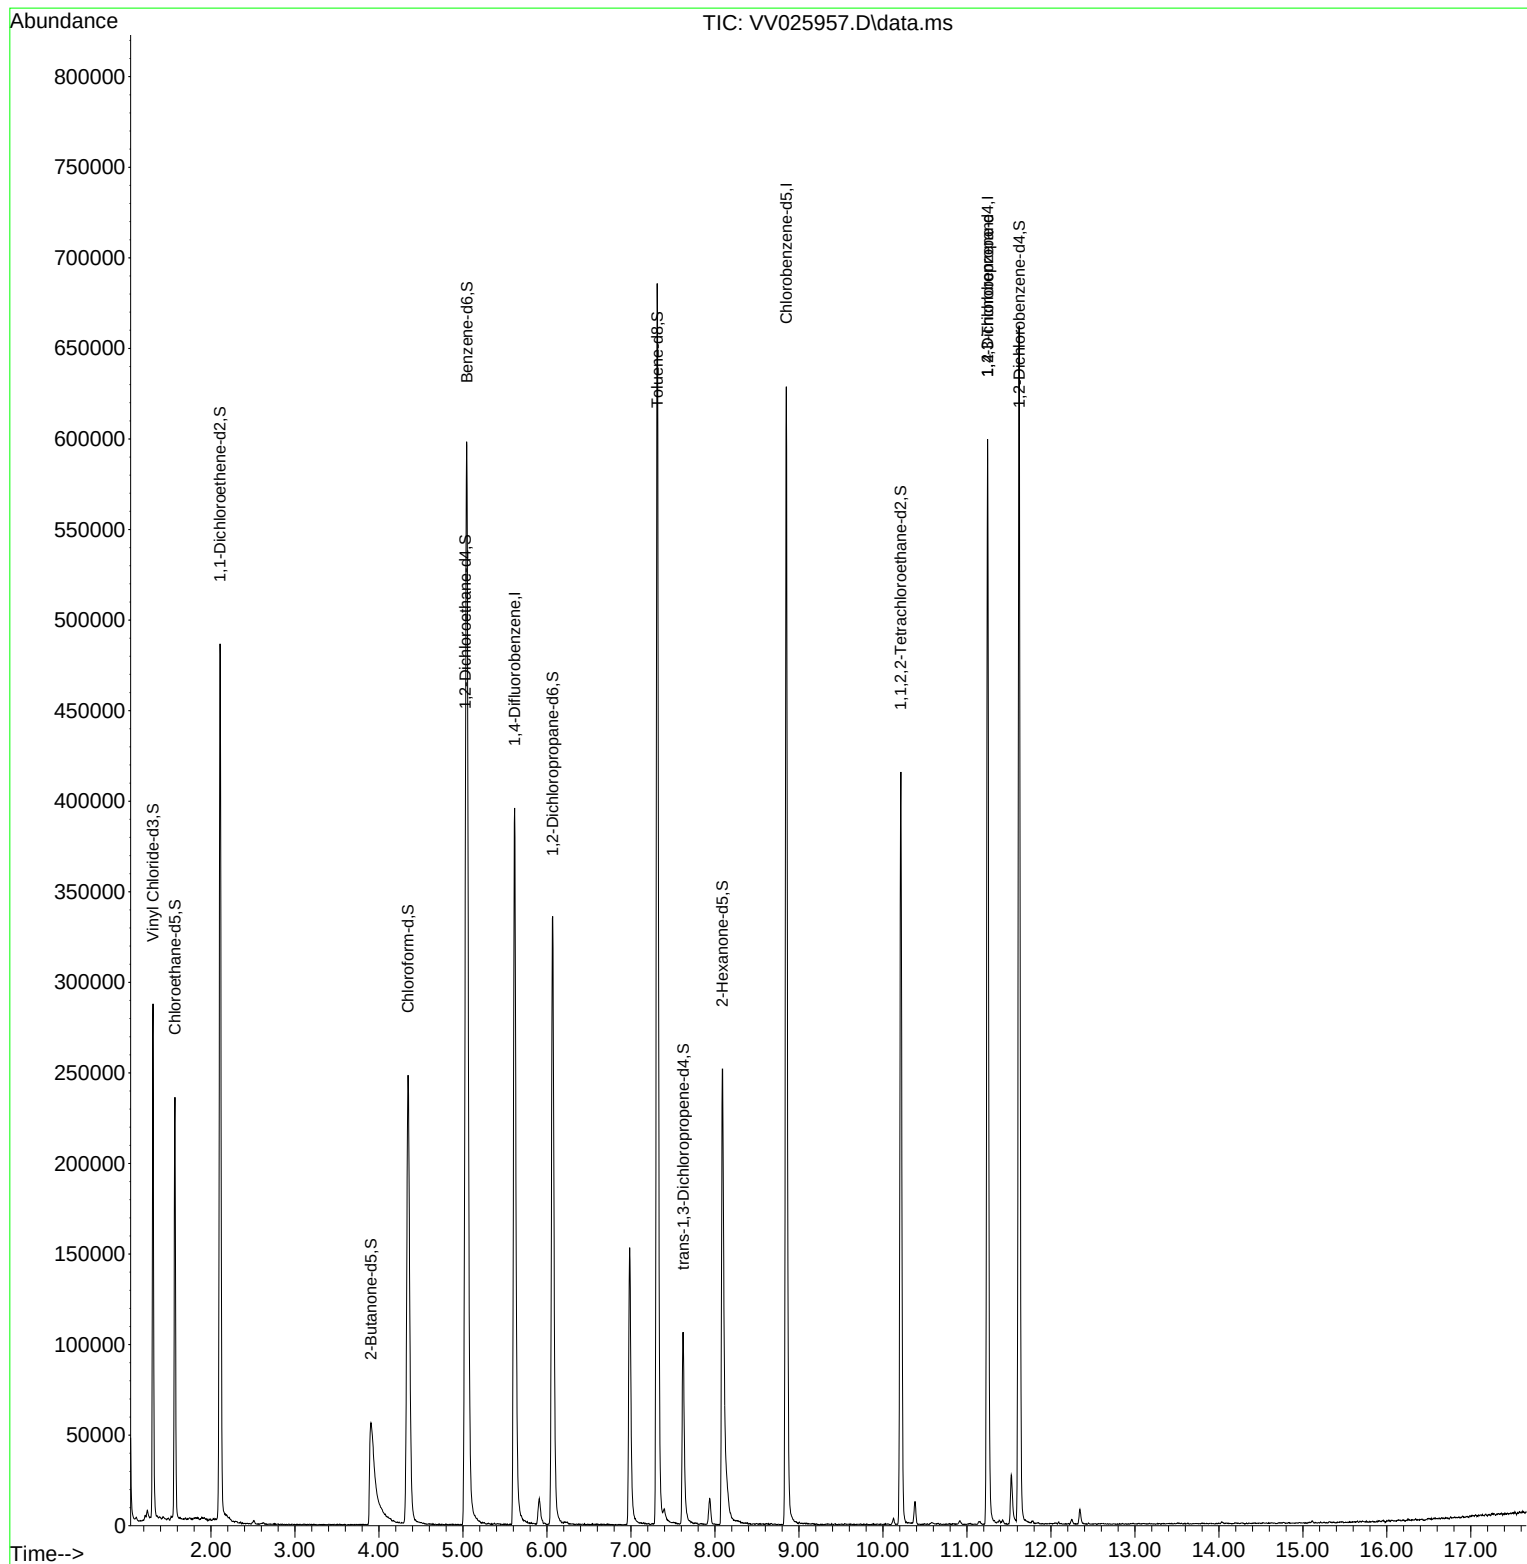

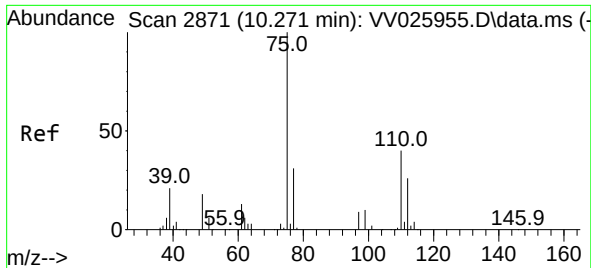

#61
 1,2,3-Trichloropropane
 Concen: 6.166 ug/L
 RT: 11.246 min Scan# 31
 Delta R.T. 0.974 min
 Lab File: VV025957.D
 Acq: 26 May 2022 14:48

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JR7

Tgt Ion: 75	Resp:	19133
Ion Ratio	Lower	Upper
75	100	
77	31.4	25.3 37.9
110	3.1	32.3 48.5#

