




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025957.D
 Acq On : 26 May 2022 14:48
 Operator : SY/MD
 Sample : N3039-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JR7

Manual IntegrationsAPPROVED

Quant Time: May 27 01:29:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 01:28:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/27/2022
 Supervised By :Mahesh Dadoda 05/27/2022

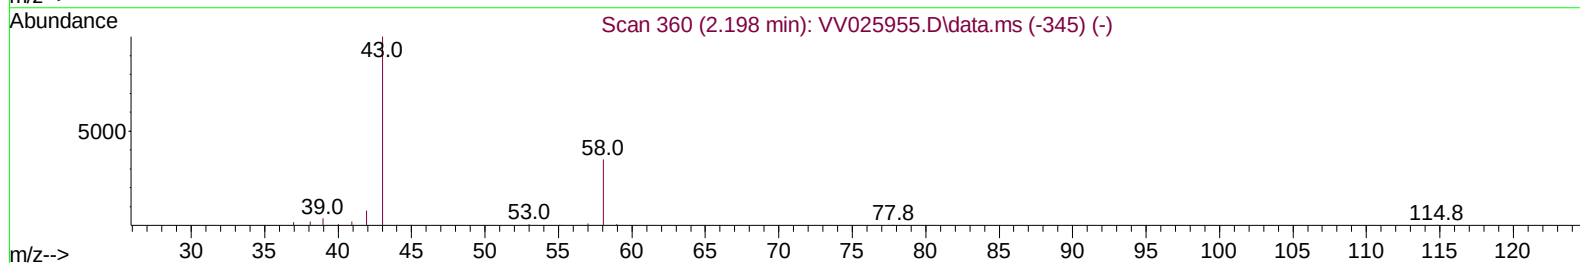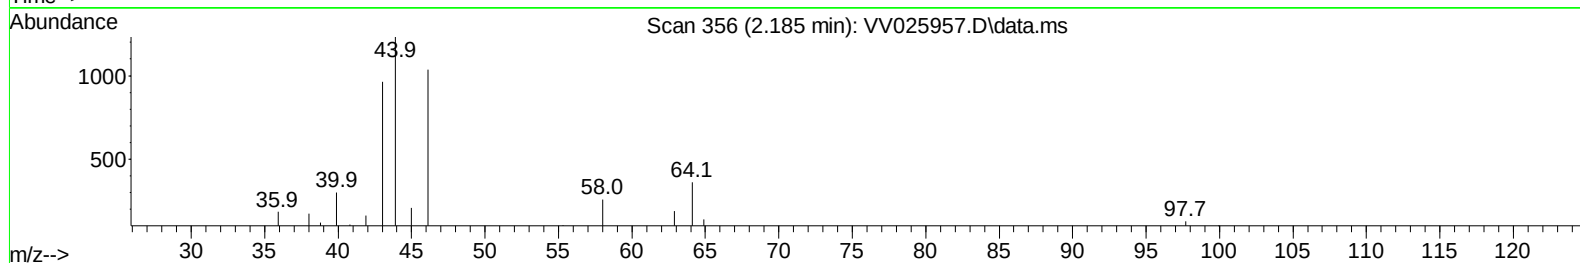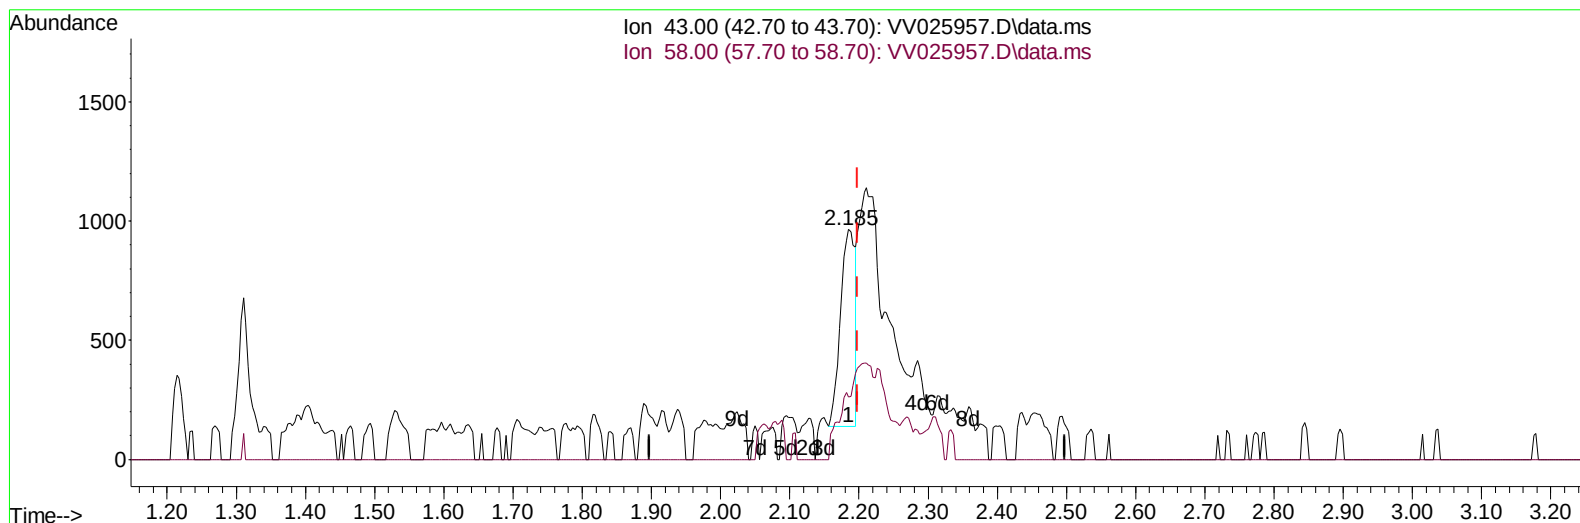

TIC: VV025957.D\data.ms

(13) Acetone (T)

2.185min (-0.013) 0.92 ug/L

response 1196

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	8.70
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025957.D
 Acq On : 26 May 2022 14:48
 Operator : SY/MD
 Sample : N3039-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JR7

Manual IntegrationsAPPROVED

Quant Time: May 27 01:29:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 01:28:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/27/2022
 Supervised By :Mahesh Dadoda 05/27/2022

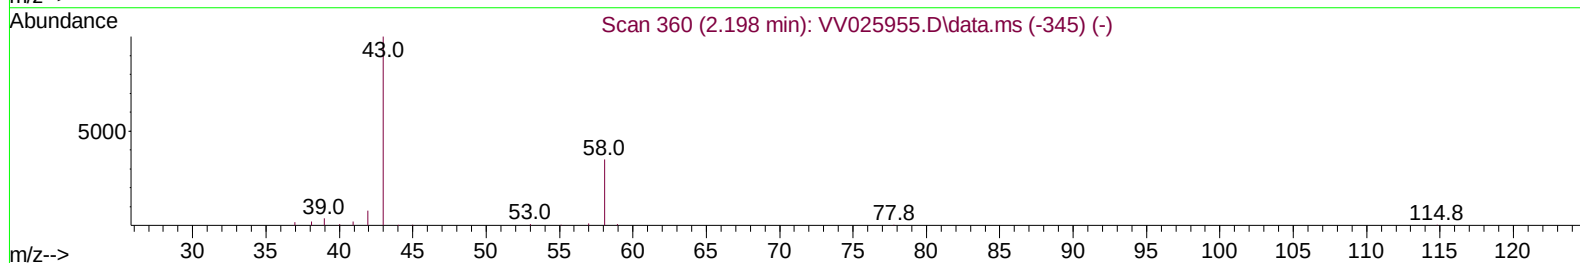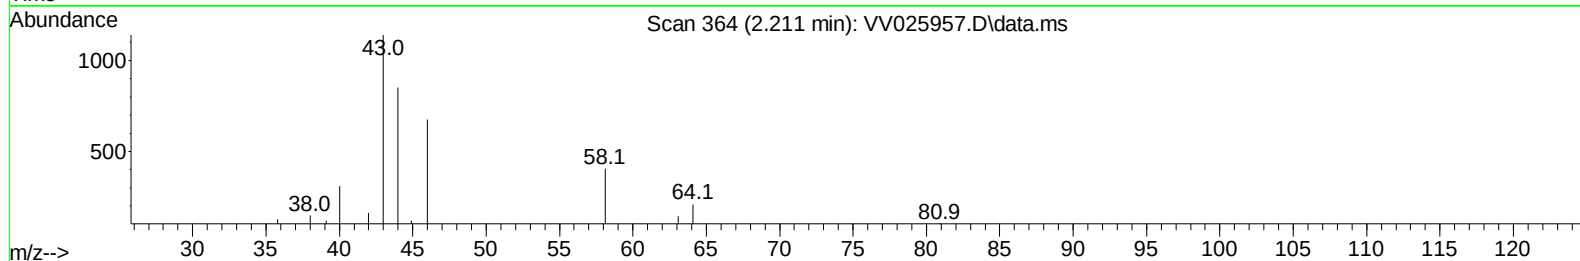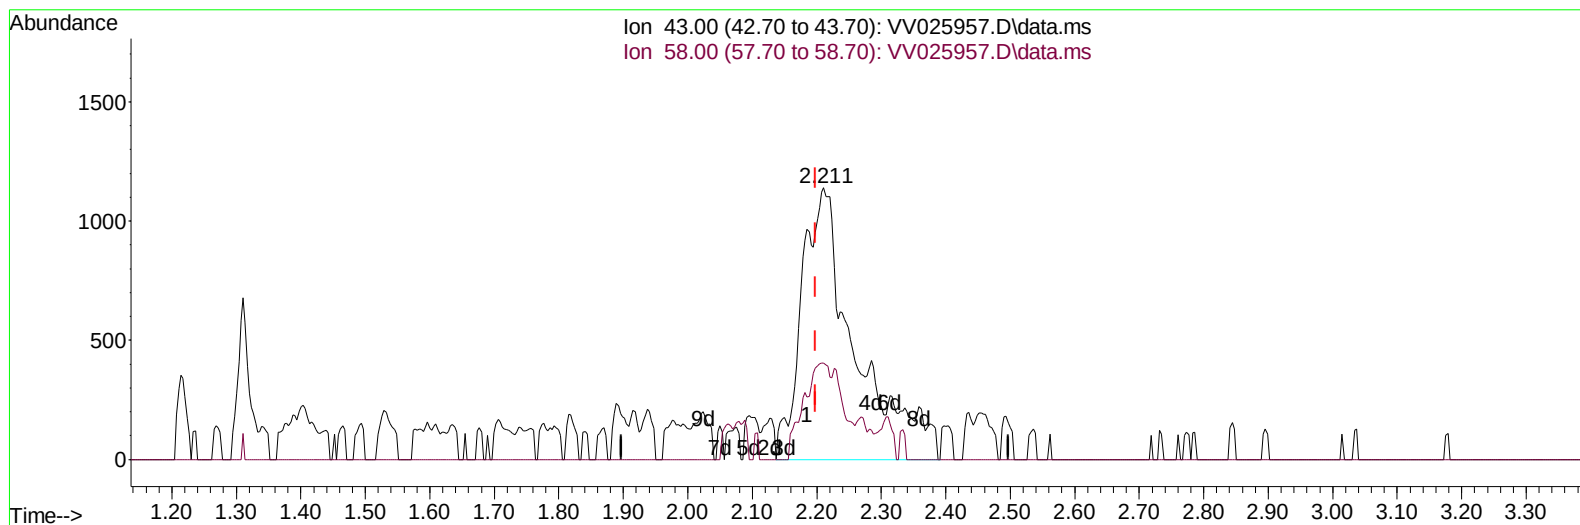

TIC: VV025957.D\data.ms

(13) Acetone (T)

2.211min (+ 0.013) 5.03 ug/L m

response 6549

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	1.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
 Data File : VV025957.D
 Acq On : 26 May 2022 14:48
 Operator : SY/MD
 Sample : N3039-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JR7

Manual IntegrationsAPPROVED

Quant Time: May 27 01:53:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 27 01:28:09 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/27/2022
 Supervised By :Mahesh Dadoda 05/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	345041	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	347382	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	156764	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	181104	40.669	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	81.340%	
7) Chloroethane-d5	1.571	69	147067	37.607	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	75.220%	
11) 1,1-Dichloroethene-d2	2.108	63	257469	33.059	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	66.120%	
21) 2-Butanone-d5	3.905	46	123536	64.725	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	64.720%	
24) Chloroform-d	4.346	84	260893	41.946	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.900%	
26) 1,2-Dichloroethane-d4	5.031	65	160753	42.764	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	85.520%	
32) Benzene-d6	5.047	84	534508	44.137	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.280%	
36) 1,2-Dichloropropane-d6	6.066	67	167378	45.000	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	90.000%	
41) Toluene-d8	7.313	98	460360	41.258	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.520%	
43) trans-1,3-Dichloroprop...	7.622	79	62893	37.879	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	75.760%	
47) 2-Hexanone-d5	8.088	63	92698	67.977	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	67.980%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	202745	40.874	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	81.740%	
66) 1,2-Dichlorobenzene-d4	11.622	152	166213	48.336	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	96.680%	
Target Compounds						
13) Acetone	2.211	43	6549m	5.028	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052622\
Data File : VV025957.D
Acq On : 26 May 2022 14:48
Operator : SY/MD
Sample : N3039-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JR7

Manual IntegrationsAPPROVED

Quant Time: May 27 01:53:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 27 01:28:09 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/27/2022
Supervised By :Mahesh Dadoda 05/27/2022

